

Sample Name :Antioxidant peptide A
 Cat. No. : RP20495
 Lot. No. : E9094619I
 Time Processed :7:14:19
 Month-Day-Year Processed : 10/07/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

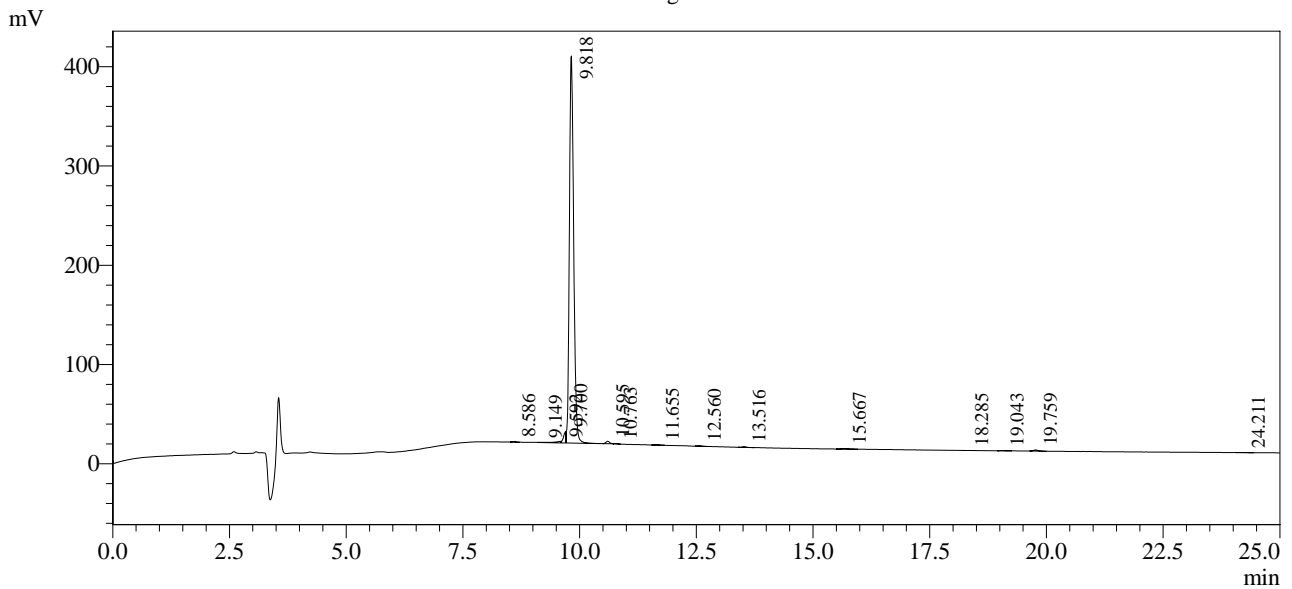

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.586	1960	430	0.075
2	9.149	2274	214	0.087
3	9.592	14020	1488	0.538
4	9.700	43072	11276	1.652
5	9.818	2503317	390145	95.999
6	10.595	13113	2406	0.503
7	10.763	1245	271	0.048
8	11.655	2742	424	0.105
9	12.560	3524	527	0.135
10	13.516	4400	725	0.169
11	15.667	5052	473	0.194
12	18.285	1603	234	0.061
13	19.043	1498	235	0.057
14	19.759	8531	1195	0.327
15	24.211	1307	138	0.050
Total		2607659	410181	100.000