

Sample Name :Flagelin22
 Cat No.: RP19986
 Lot No.:E9682319J
 Time Processed :8:27:39
 Month-Day-Year Processed :10/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

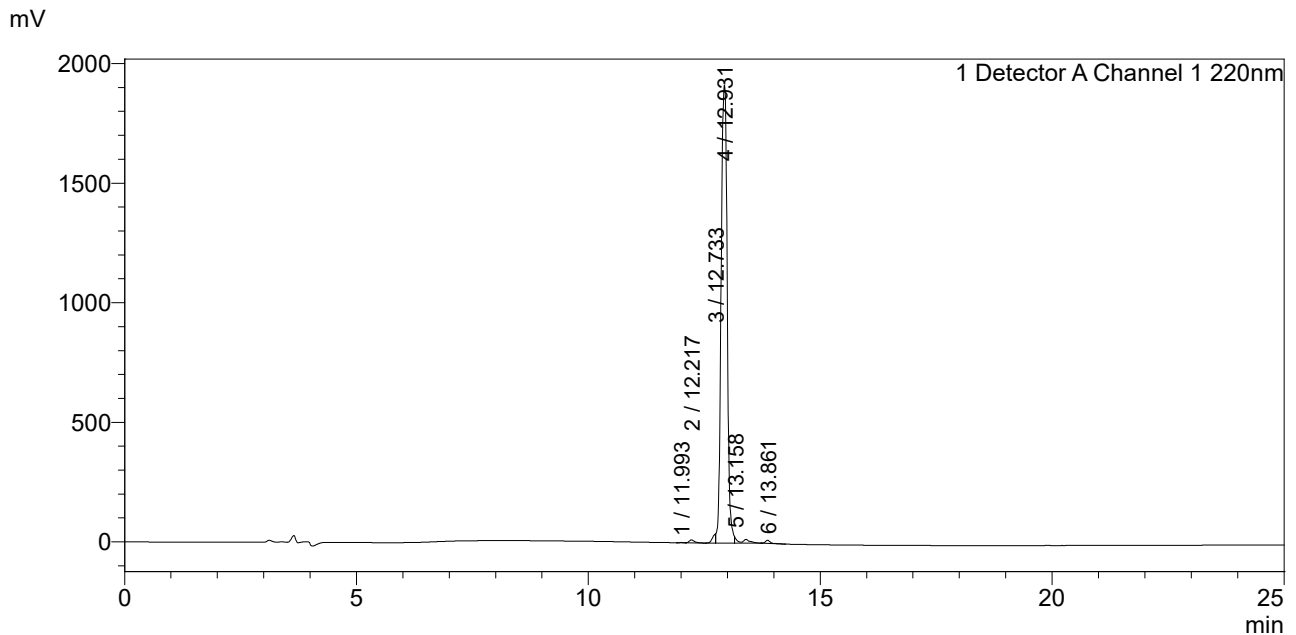

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.993	3579	646	0.020
2	12.217	95481	12065	0.532
3	12.733	177762	37230	0.990
4	12.931	17353603	1915698	96.625
5	13.158	236735	24380	1.318
6	13.861	92564	13150	0.515
Total		17959724	2003170	100.000