

Sample Name :Octreotide (SMS 201-995)

Sample ID :U5688CI250-1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

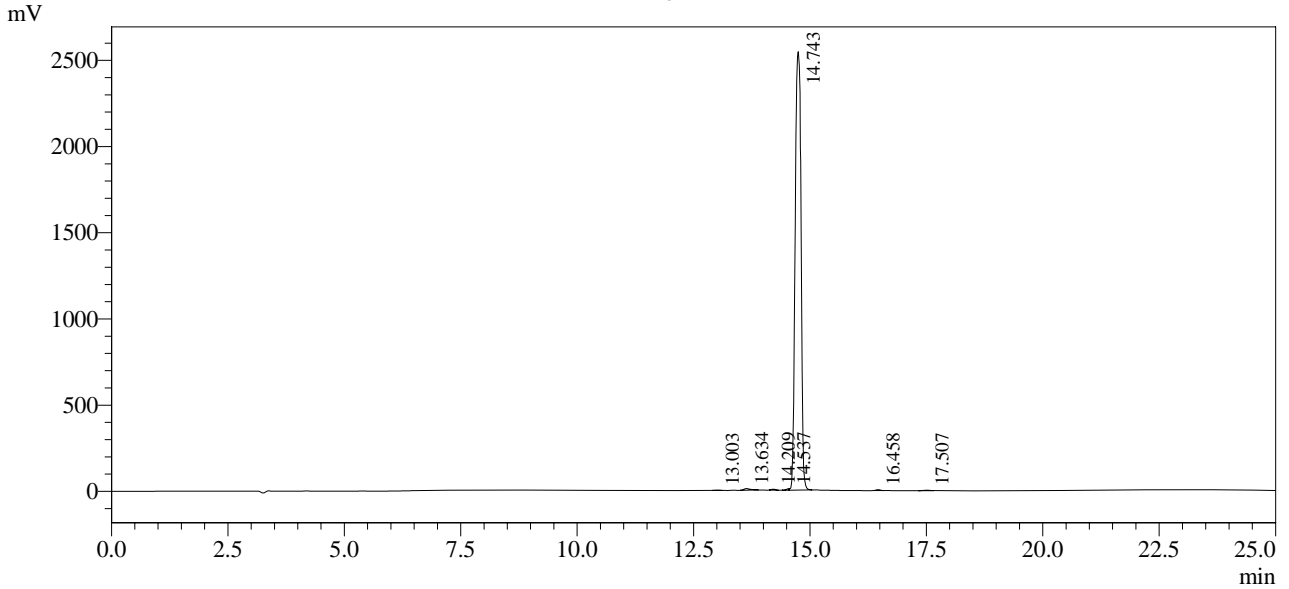

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.003	5879	835	0.026
2	13.634	89995	9376	0.402
3	14.209	30210	5067	0.135
4	14.537	32304	8025	0.144
5	14.743	22162642	2542434	99.053
6	16.458	28021	4541	0.125
7	17.507	25535	2468	0.114
Total		22374586	2572745	100.000