

Sample Name :MUC5AC  
 Cat No.: RP20290  
 Lot No.:E5806720C  
 Time Processed :16:48:23  
 Month-Day-Year Processed :03/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

| Time  | Module     | Command       | Value |
|-------|------------|---------------|-------|
| 0.01  | Pumps      | Pump A B.Conc | 15    |
| 25.00 | Pumps      | Pump A B.Conc | 65    |
| 25.01 | Pumps      | Pump A B.Conc | 95    |
| 32.00 | Pumps      | Pump A B.Conc | 95    |
| 50.00 | Pumps      | Pump A B.Conc | 5     |
| 51.00 | Pumps      | Pump A B.Conc | 5     |
| 55.00 | Controller | Stop          |       |


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

mV

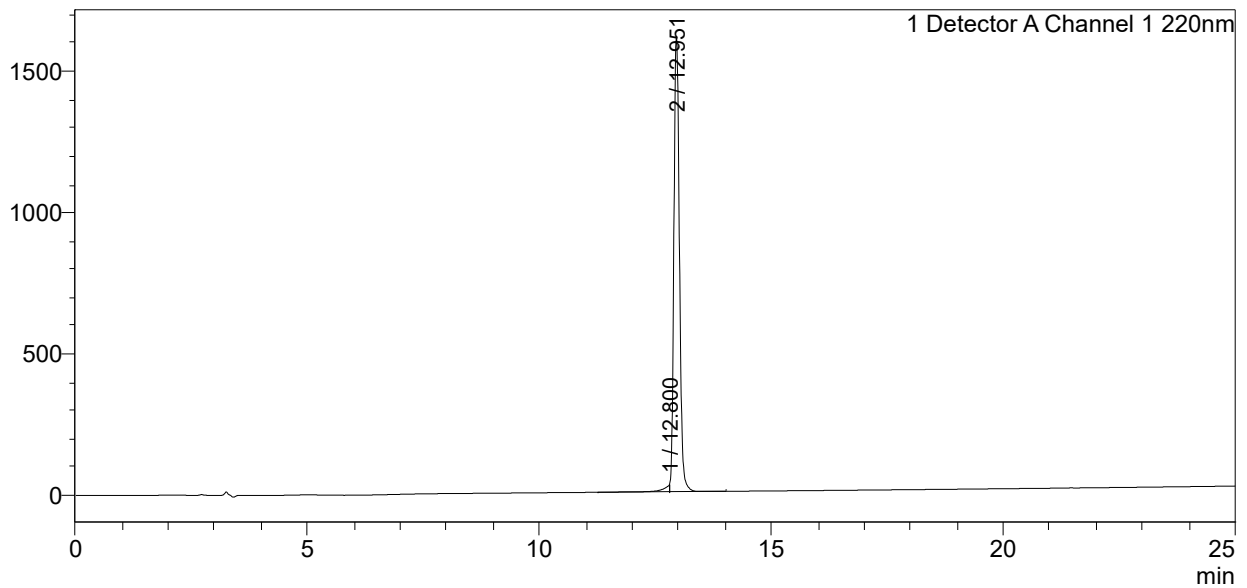

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area     | Height  | Area%   |
|-------|-----------|----------|---------|---------|
| 1     | 12.800    | 223905   | 24362   | 1.648   |
| 2     | 12.951    | 13364218 | 1612585 | 98.352  |
| Total |           | 13588123 | 1636947 | 100.000 |