

Sample Name : Angiotensin I, human
 Cat. No. : RP11251
 Lot. No. : E1187419F
 Time Processed : 9:29:42
 Month-Day-Year Processed : 06/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

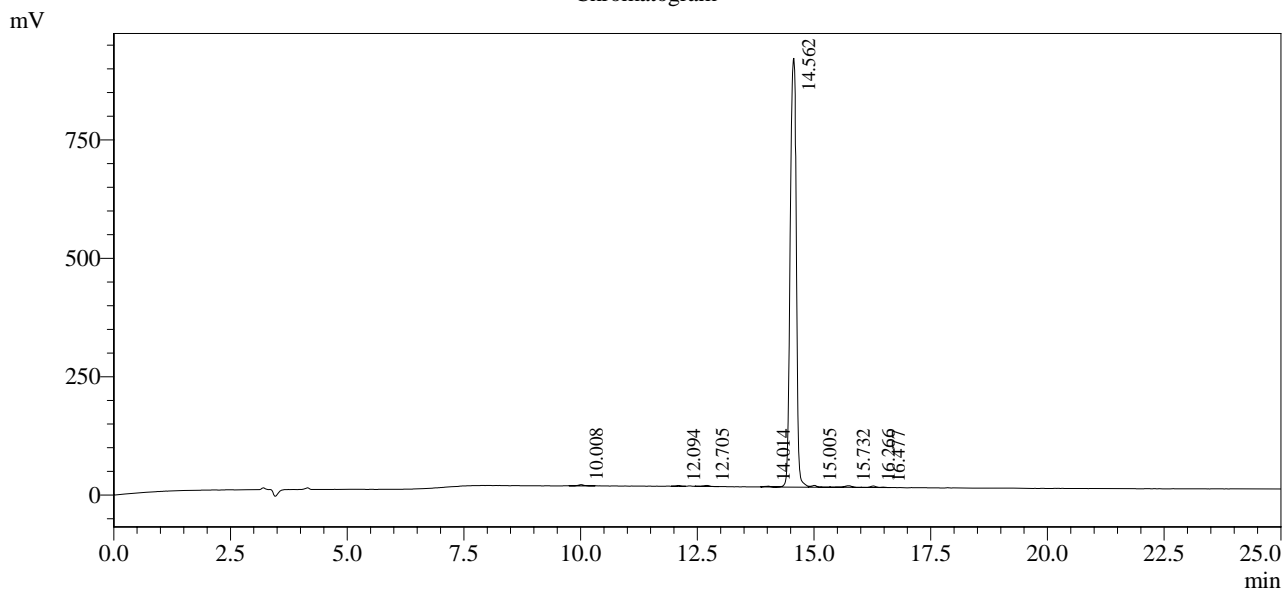

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.008	28730	2704	0.342
2	12.094	9690	1424	0.115
3	12.705	19747	2060	0.235
4	14.014	14221	1557	0.169
5	14.562	8226043	905517	97.830
6	15.005	33376	3790	0.397
7	15.732	43351	3476	0.516
8	16.266	27563	3220	0.328
9	16.477	5746	898	0.068
Total		8408466	924645	100.000