

Sample Name :OVA Peptide(257-264)  
 Cat. No. :RP10611  
 Lot. No. :PE2201708

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

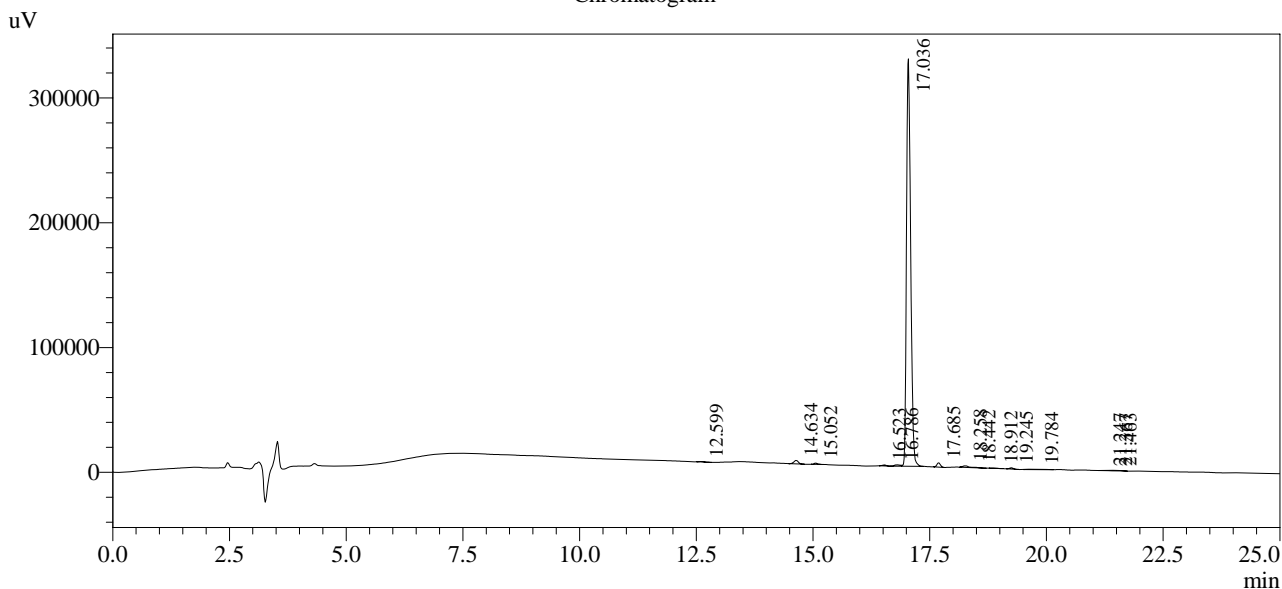

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.599	2540	393	0.119
2	14.634	18853	2804	0.886
3	15.052	5755	1055	0.271
4	16.523	4392	750	0.207
5	16.786	10037	1101	0.472
6	17.036	2026187	326423	95.275
7	17.685	18276	3410	0.859
8	18.258	9975	1260	0.469
9	18.442	3653	409	0.172
10	18.912	3032	371	0.143
11	19.245	5394	969	0.254
12	19.784	9222	469	0.434
13	21.247	2637	318	0.124
14	21.367	1481	343	0.070
15	21.463	5236	445	0.246
Total		2126670	340520	100.000