

Sample Name: Bactenecin, bovine

Cat. No. : RP11235

Lot. No. : E9586919L

Time Processed: 12:30:00 PM

Month-Day-Year Processed :01/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Equipment: ZJ19010325

<Chromatogram>

mV

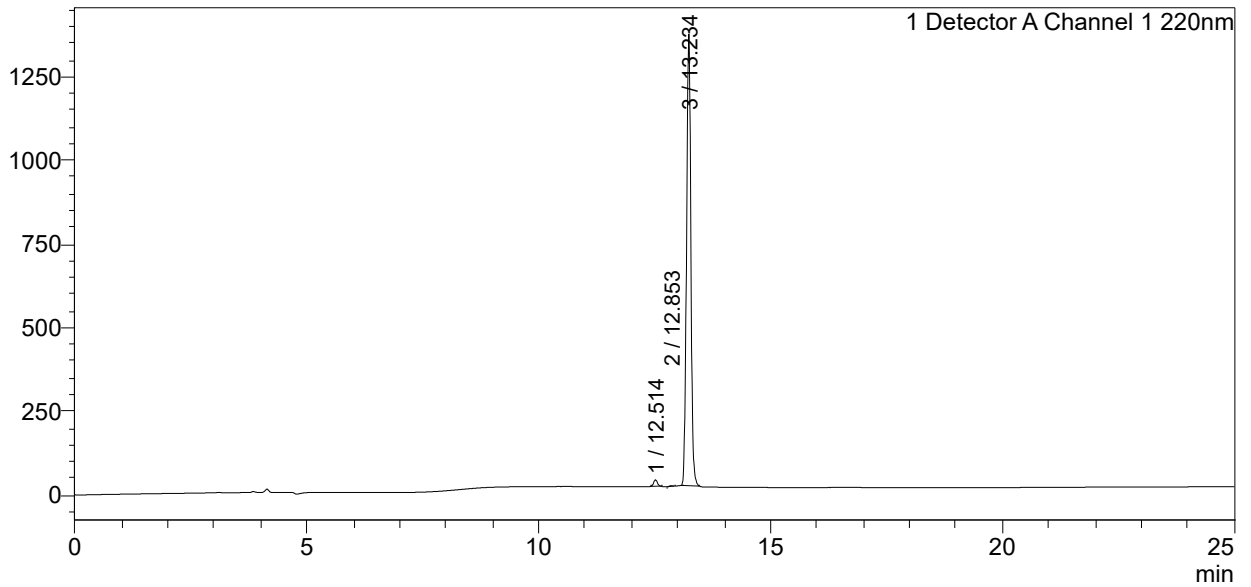

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.514	109318	19914	1.233
2	12.853	6965	1513	0.079
3	13.234	8750867	1347764	98.689
Total		8867150	1369191	100.000