


# Mass Spectrum

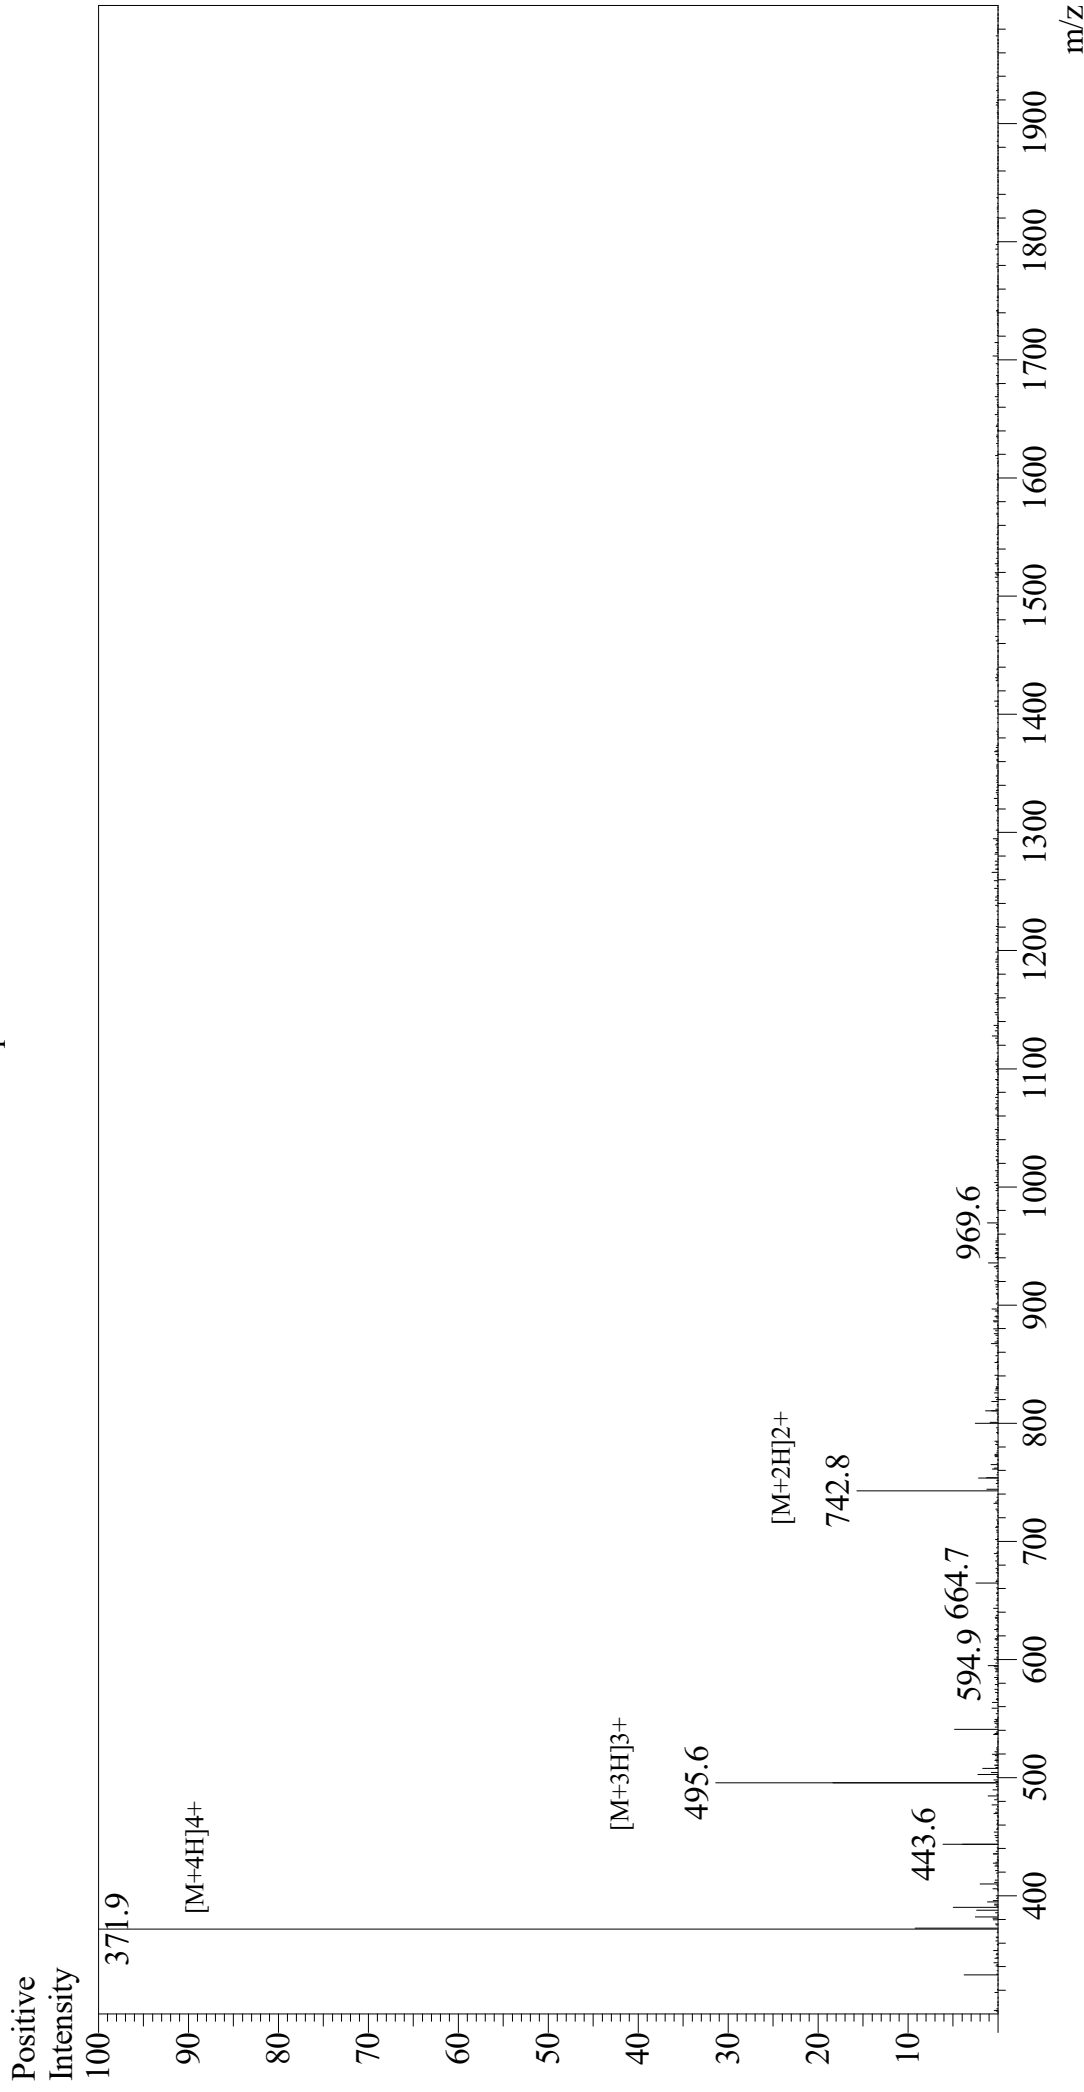

## Sample Information

Acquired by : Gary  
 Month-Day Processed : 01/29/20  
 Time Processed : 09:33:42 AM  
 Injection Volume : 0.3  
 Sample Name : Bactenecin, bovine  
 Cat. No. : RP11235  
 Lot. No. : E9586919L  
 Theoretical MW : 1483.90  
 Observed MW : 1483.6

Interface : ESI  
 Nebulizing Gas Flow : 1.5L/min  
 CDL Temp : 250  
 Block Temp : 200

Equipment : GK11010007  
 Interface Bias : +4.5 kV  
 Drying Gas Flow : 5 L/min  
 T.Flow : 0.2 ml/min  
 B.conc : 50% H<sub>2</sub>O/50% MeOH