

Sample Name : Kisspeptin-10  
 Cat. No. : RP20494  
 Lot. No. : PE6051812  
 Time Processed :20:00:06  
 Month-Day-Year Processed :12/05/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

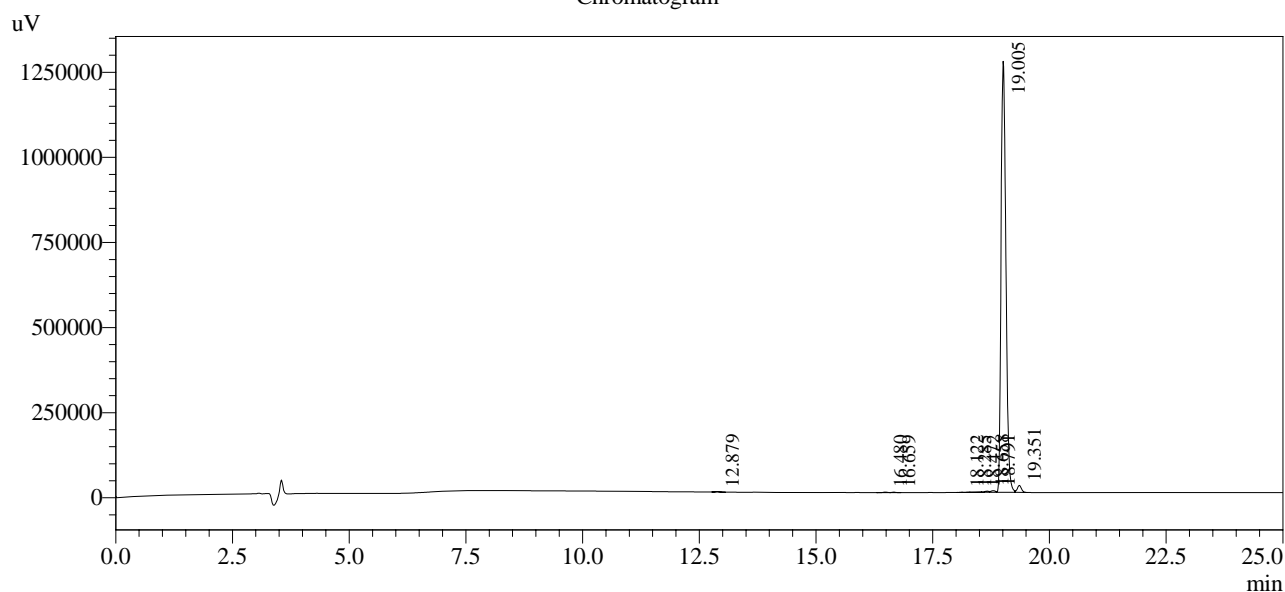

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.879	9491	1712	0.101
2	16.480	9601	1590	0.103
3	16.659	8442	1441	0.090
4	18.122	4073	713	0.044
5	18.285	7870	876	0.084
6	18.472	1286	255	0.014
7	18.658	19236	3311	0.206
8	18.791	30984	4768	0.331
9	19.005	9139253	1266312	97.703
10	19.351	123889	20307	1.324
Total		9354123	1301285	100.000