

Sample Name: C-Type Natriuretic Peptide (CNP) (1-22), human

Cat. No. : RP11110

Lot. No. : E0601719L

Time Processed: 14:11:33

Month-Day-Year Processed :12/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Equipment:ZJ19010324

### <Chromatogram>

mV

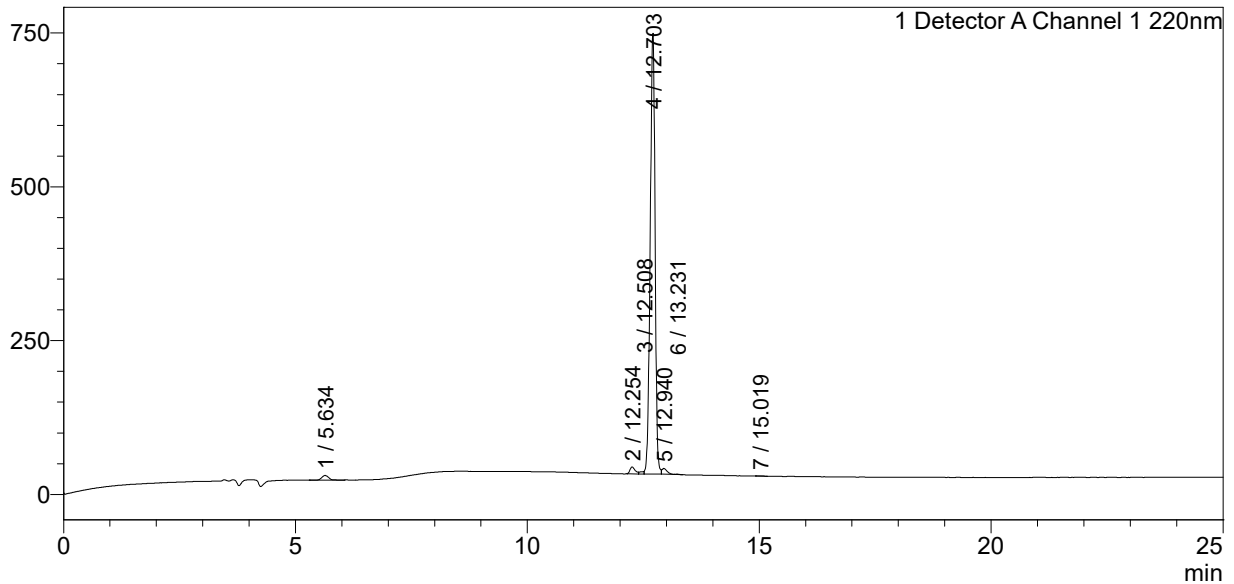

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.634	77350	7565	1.414
2	12.254	87064	11367	1.592
3	12.508	25235	3962	0.461
4	12.703	5205241	716836	95.163
5	12.940	69429	9422	1.269
6	13.231	2760	569	0.050
7	15.019	2752	367	0.050
Total		5469831	750088	100.000