

Sample Name :Hepatitis B Virus Core (128-140)
 Cat No. : RP17313
 Lot No. : E3625120B
 Time Processed : 12:02:19
 Month-Day-Year Processed : 02/08/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
41.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

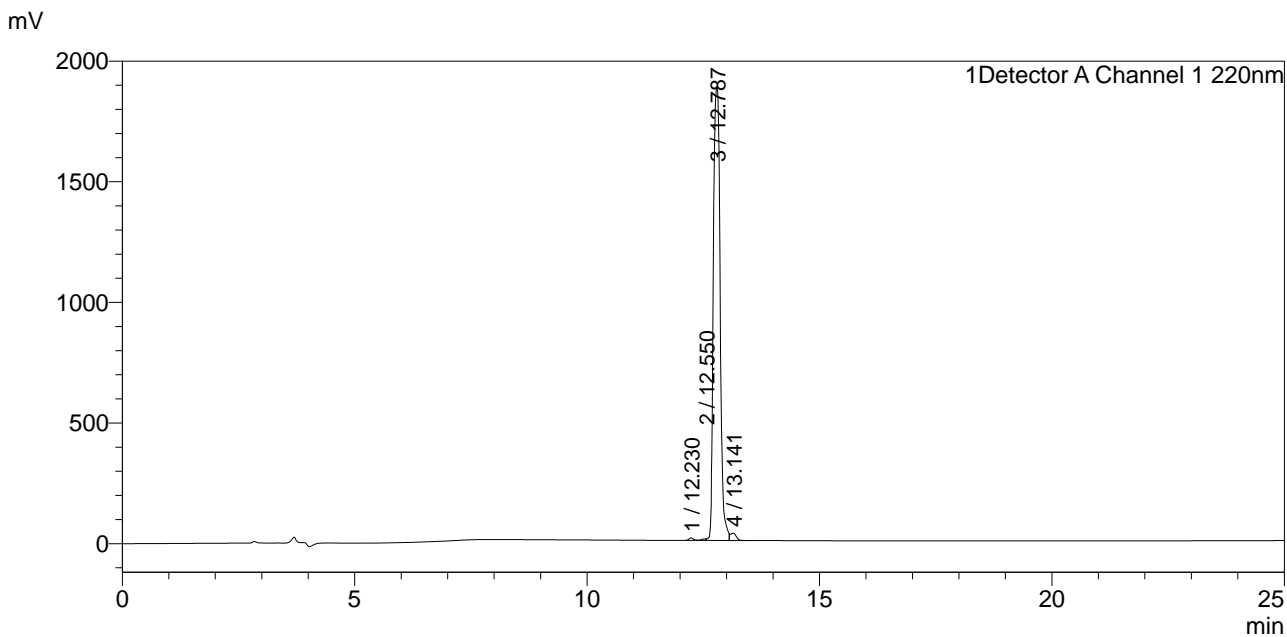

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.230	63224	10652	0.328
2	12.550	40446	5967	0.210
3	12.787	18899449	1880009	98.058
4	13.141	270591	30048	1.404
Total		19273711	1926675	100.000