

Sample Name :Glycoprotein (276-286)
 Cat No. :RP19983
 Lot No. :E4830419I
 Time Processed :7:41:54
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

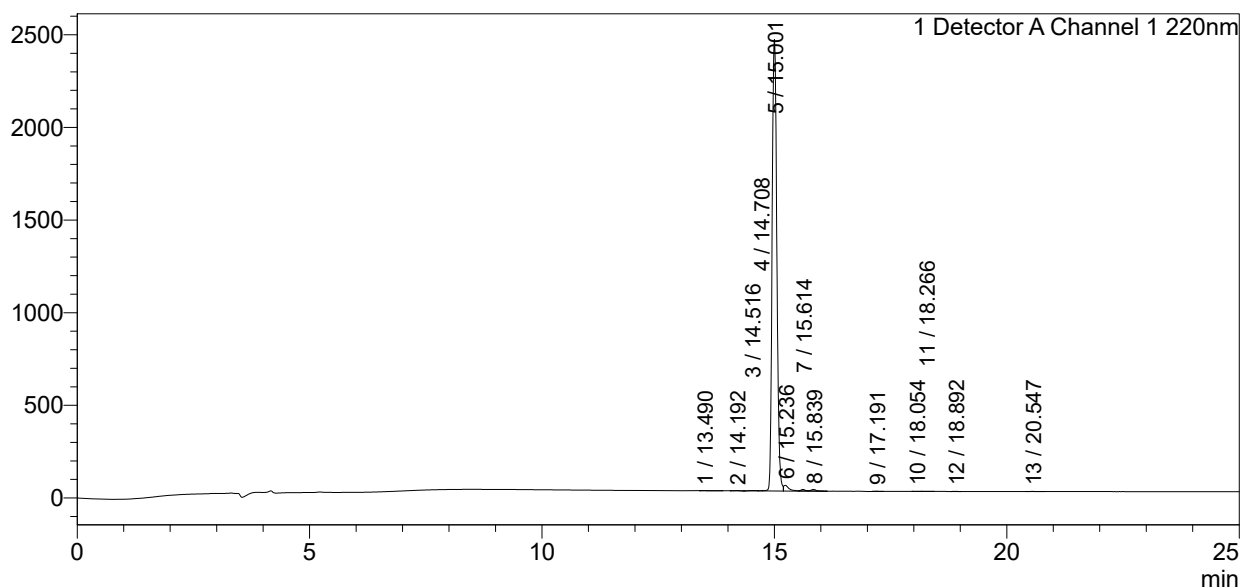

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.490	6751	960	0.039
2	14.192	8707	1427	0.050
3	14.516	21777	1924	0.125
4	14.708	7412	1464	0.042
5	15.001	17056505	2437203	97.544
6	15.236	261705	30724	1.497
7	15.614	46011	8080	0.263
8	15.839	62697	8665	0.359
9	17.191	2152	367	0.012
10	18.054	2354	379	0.013
11	18.266	2604	380	0.015
12	18.892	1515	273	0.009
13	20.547	5797	730	0.033
Total		17485989	2492576	100.000