

Sample Name : Arg-Gly-Glu-Ser  
 Cat. No. : RP13448  
 Lot. No. : E3605519K  
 Time Processed :20:40:12  
 Month-Day-Year Processed :11/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	0	
5.00	Pumps	Pump A B.Conc	0	
20.00	Pumps	Pump A B.Conc	30	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	0	
40.00	Pumps	Pump A B.Conc	0	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

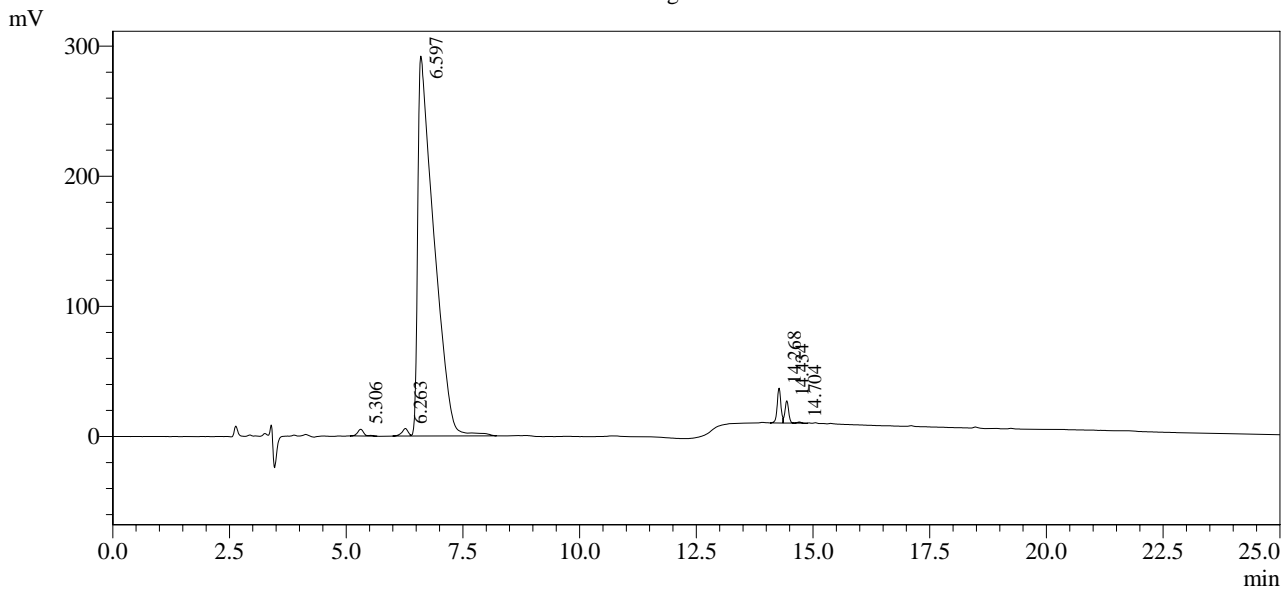

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.306	49618	5225	0.672
2	6.263	53544	5822	0.725
3	6.597	7037002	292032	95.253
4	14.268	148644	26734	2.012
5	14.434	93709	17113	1.268
6	14.704	5170	896	0.070
Total		7387688	347822	100.000