

Sample Name : InfluenzaHA.518-526.

Cat. No. : RP20284 Lot. No. : PE7671801

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

### Chromatogram

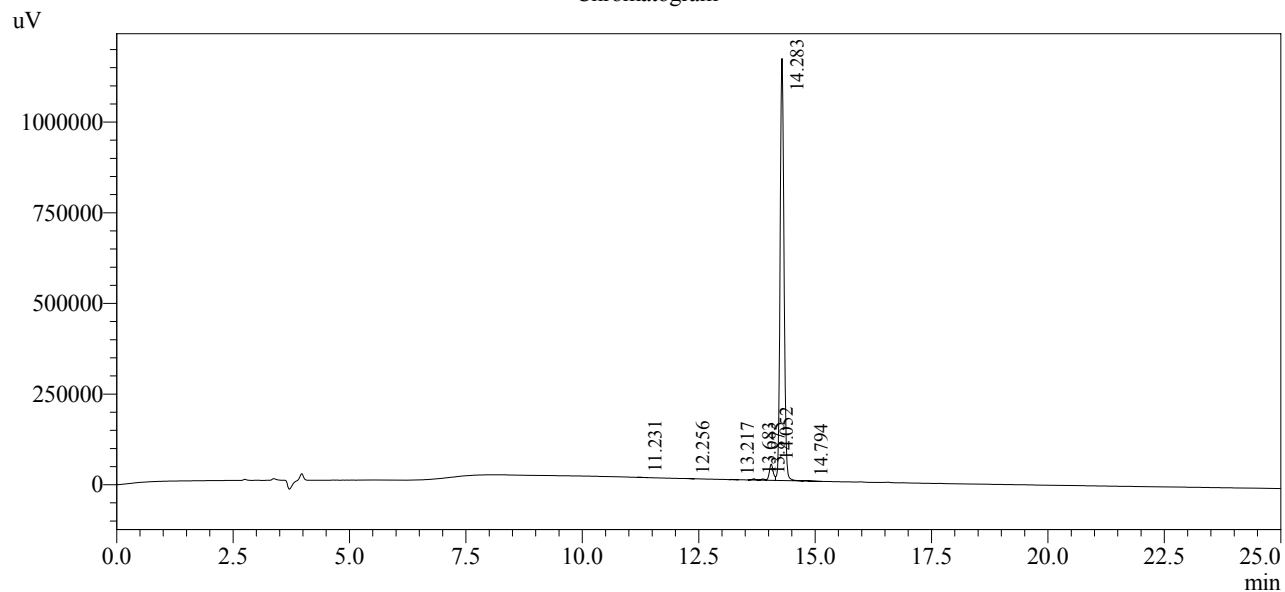

1 Det.A Ch1 / 220nm

### Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.231	2247	459	0.032
2	12.256	2762	558	0.039
3	13.217	1838	316	0.026
4	13.683	16869	3225	0.238
5	13.875	17864	3303	0.252
6	14.052	261931	44749	3.692
7	14.283	6780866	1163408	95.575
8	14.794	10447	1331	0.147
Total		7094824	1217349	100.000