

Sample Name : N-Boc-Phe-Leu-Phe-Leu-Phe
 Cat. No. : RP12950
 Lot. No. : PE5811806

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	35	
25.00	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	35	
40.00	Pumps	Pump B Conc.	35	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Chromatogram

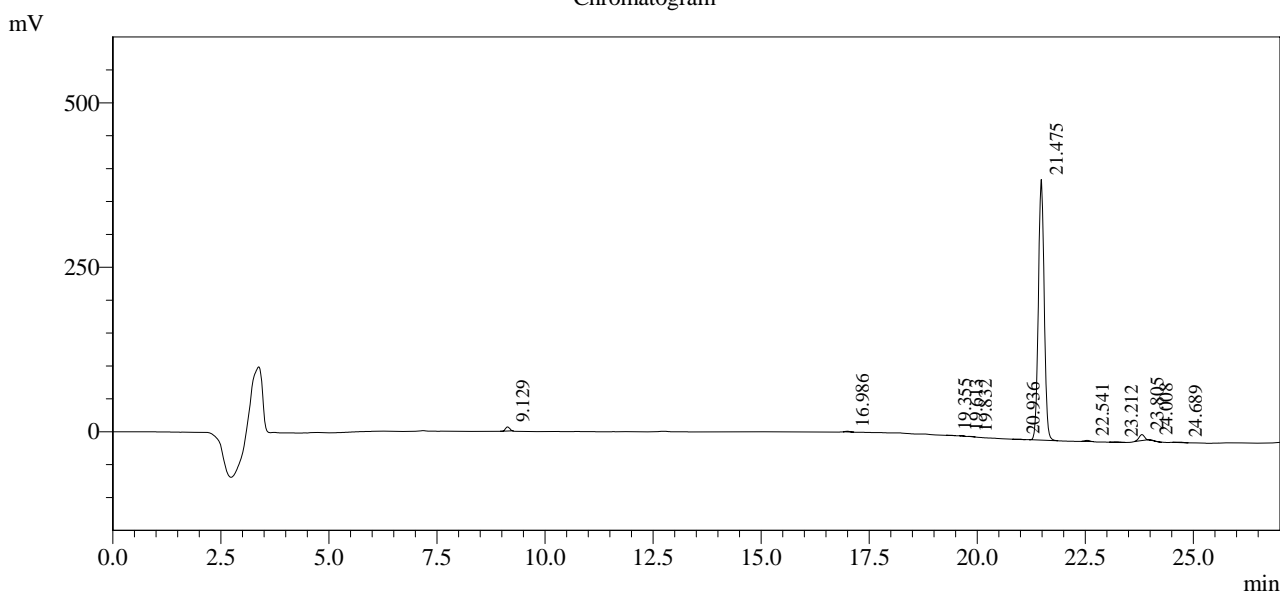

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.129	43910	6409	1.128
2	16.986	7619	1051	0.196
3	19.355	3441	543	0.088
4	19.613	889	156	0.023
5	19.832	1160	173	0.030
6	20.936	6678	740	0.171
7	21.475	3725378	396039	95.676
8	22.541	13369	1676	0.343
9	23.212	3771	403	0.097
10	23.805	80230	9164	2.060
11	24.008	884	526	0.023
12	24.689	6426	544	0.165
Total		3893754	417422	100.000