


Mass Spectrum

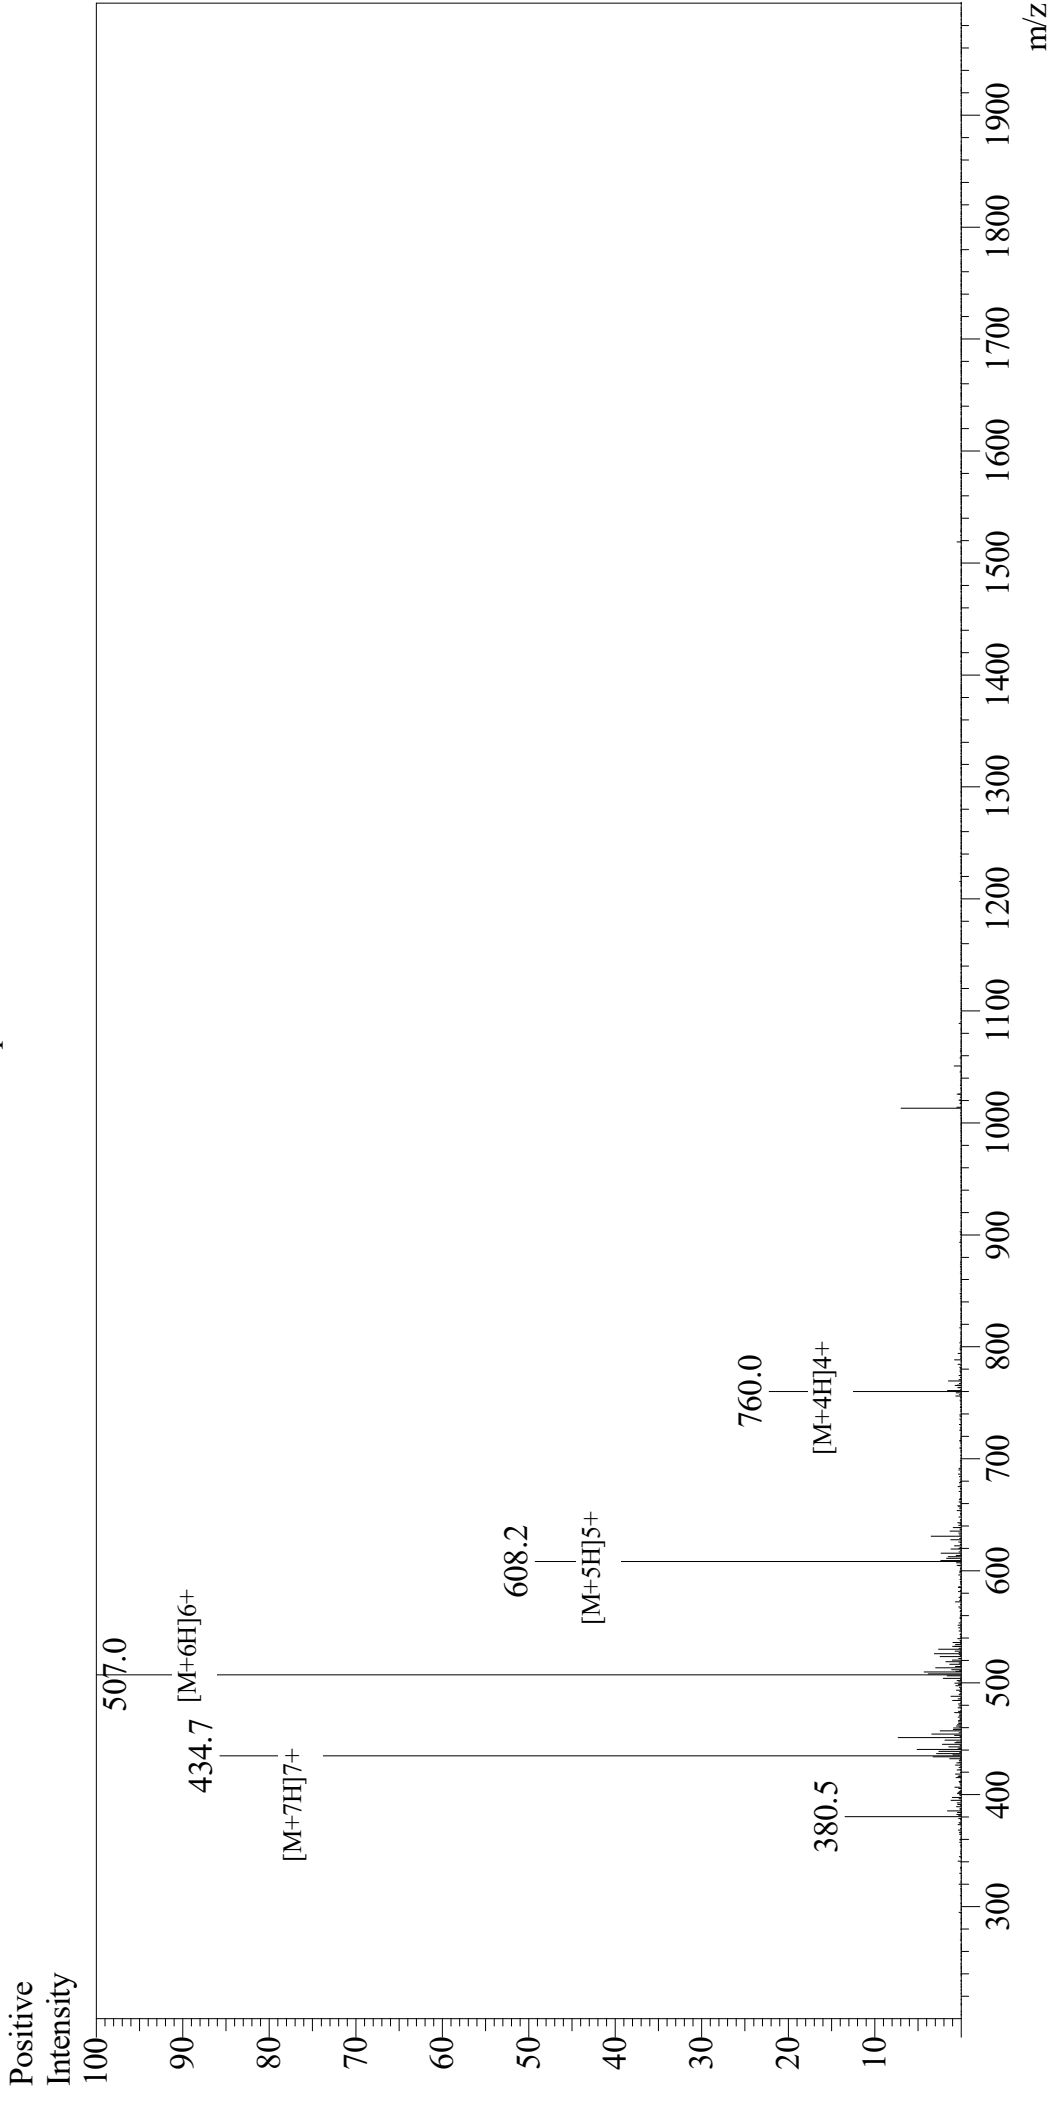

Sample Information

User :	Gary	Equipment	: GK11010007
Month-Day Processed :	10/02/19	Interface Bias	: +4.5kV
Time Processed :	06:14:29 PM	Drying Gas Flow	: 5 L/min
Injection Volume :	0.3	T.Flow	: 0.2ml/min
Sample Name :	Histatin 5	B.conc	: 50% H ₂ O / 50% MeOH
Cat No. :	RP11240		
Lot No. :	E7017319J		
Theoretical MW :	3036.29		
Observed MW :	3036.0		