

Sample Name: PACAP (1-38), human, ovine, rat
 Cat No. : RP10335
 Lot No. : E4728320K
 Time Processed : 6:09:23
 Month-Day-Year Processed : 11/29/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

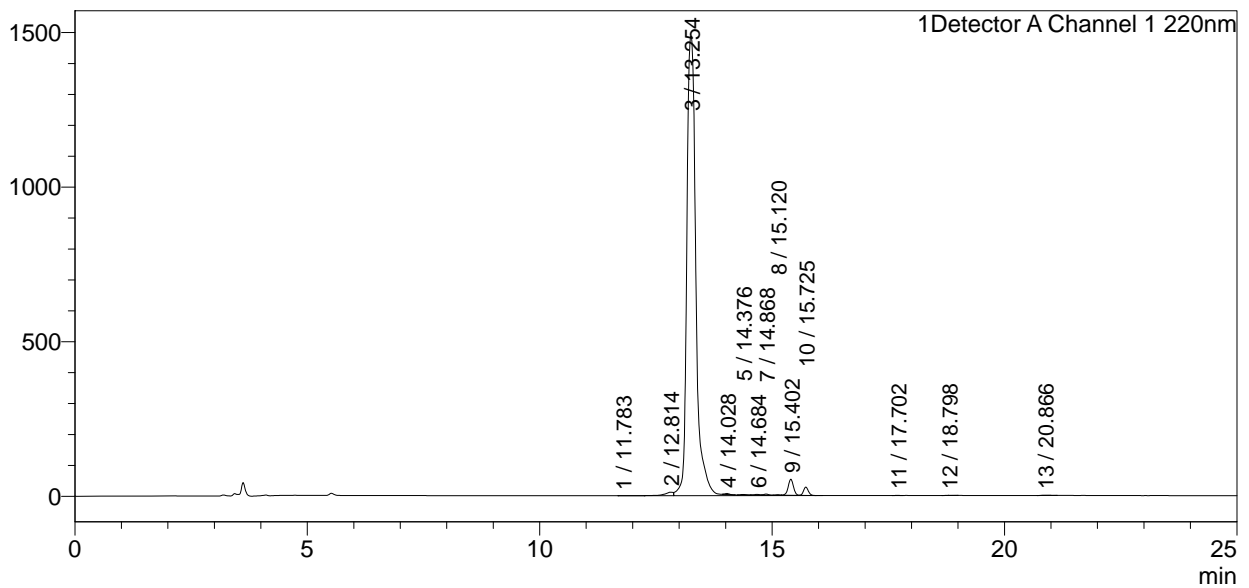

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.783	3501	239	0.017
2	12.814	148401	11408	0.704
3	13.254	20217595	1482654	95.858
4	14.028	19954	3196	0.095
5	14.376	17507	2099	0.083
6	14.684	20424	2451	0.097
7	14.868	24893	3732	0.118
8	15.120	11140	1700	0.053
9	15.402	413340	51773	1.960
10	15.725	193197	26739	0.916
11	17.702	1739	277	0.008
12	18.798	5564	635	0.026
13	20.866	13986	1098	0.066
Total		21091240	1588001	100.000