

Sample Name :Tetradecapeptide Renin Substrate, human
 Cat No. :RP20216
 Lot No. :E7093519J
 Time Processed :3:04:11 AM
 Month-Day-Year Processed :10/03/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

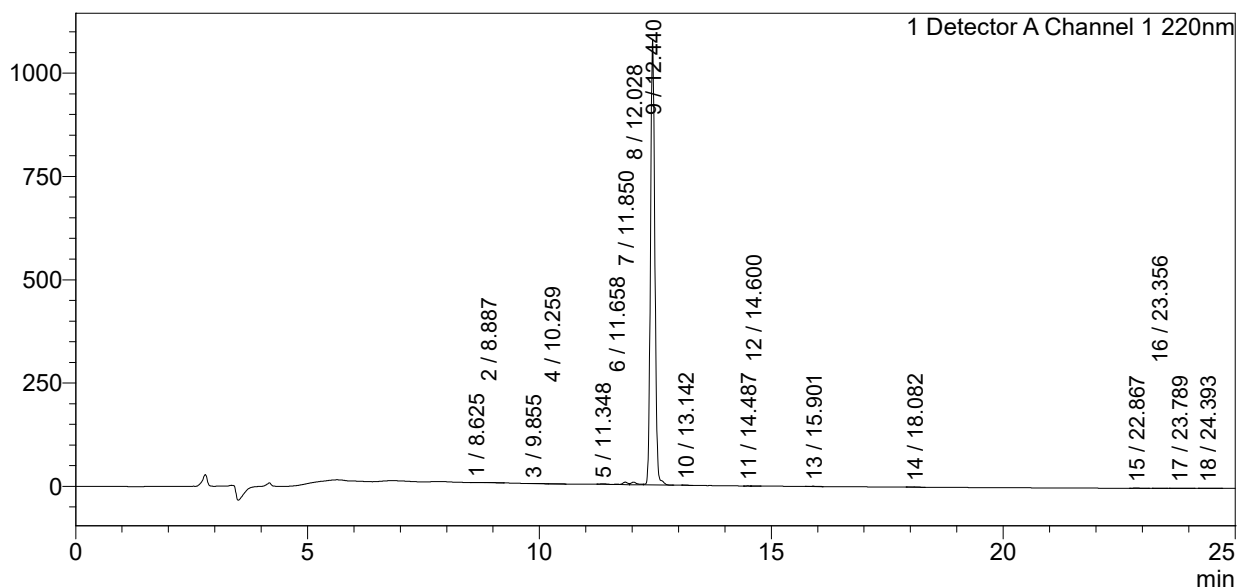

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.625	1370	146	0.019
2	8.887	4706	201	0.066
3	9.855	3611	208	0.050
4	10.259	2534	194	0.035
5	11.348	12214	1270	0.170
6	11.658	4372	635	0.061
7	11.850	42993	6132	0.600
8	12.028	56359	6129	0.786
9	12.440	7015213	1079115	97.835
10	13.142	2593	492	0.036
11	14.487	1165	194	0.016
12	14.600	1459	230	0.020
13	15.901	4834	639	0.067
14	18.082	7349	774	0.102
15	22.867	4270	404	0.060

Peak#	Ret. Time	Area	Height	Area%
16	23.356	1001	95	0.014
17	23.789	2767	201	0.039
18	24.393	1618	88	0.023
Total		7170427	1097146	100.000