

Sample Name :HEL(46-61)  
 Cat No. : RP11736  
 Lot No. :PE9641904  
 Time Processed : 7:15:16  
 Month-Day-Year Processed : 04/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

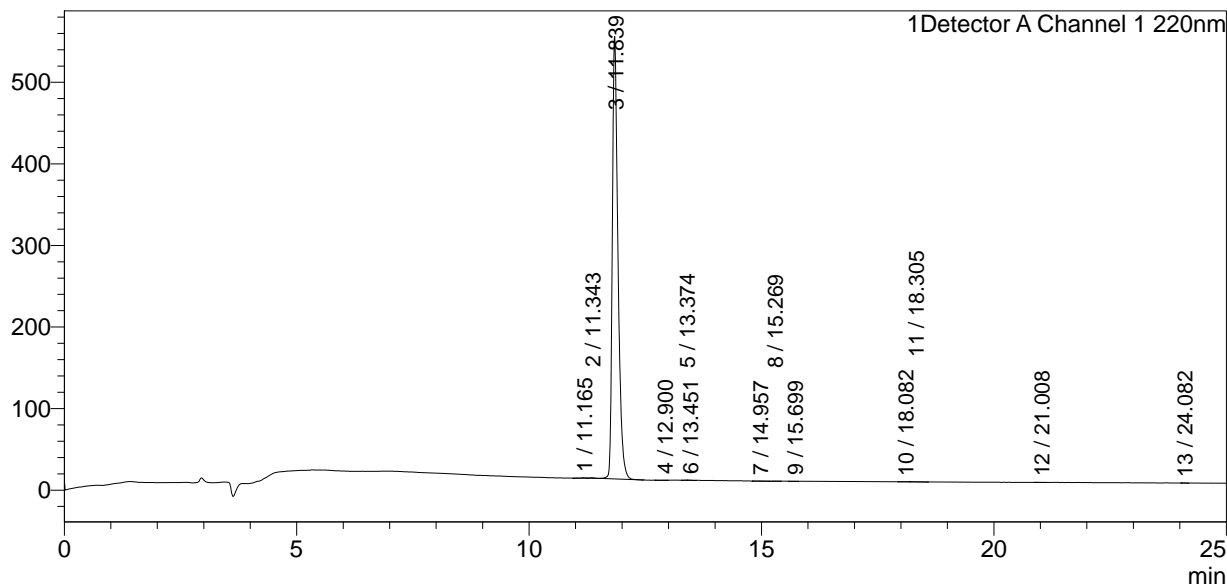

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.165	4924	539	0.106
2	11.343	5745	719	0.124
3	11.839	4601187	542398	99.365
4	12.900	1905	247	0.041
5	13.374	1324	249	0.029
6	13.451	2373	288	0.051
7	14.957	1687	161	0.036
8	15.269	1391	199	0.030
9	15.699	3105	386	0.067
10	18.082	2239	356	0.048
11	18.305	2468	252	0.053
12	21.008	1197	108	0.026
13	24.082	1058	218	0.023
Total		4630605	546119	100.000