


Mass Spectrum

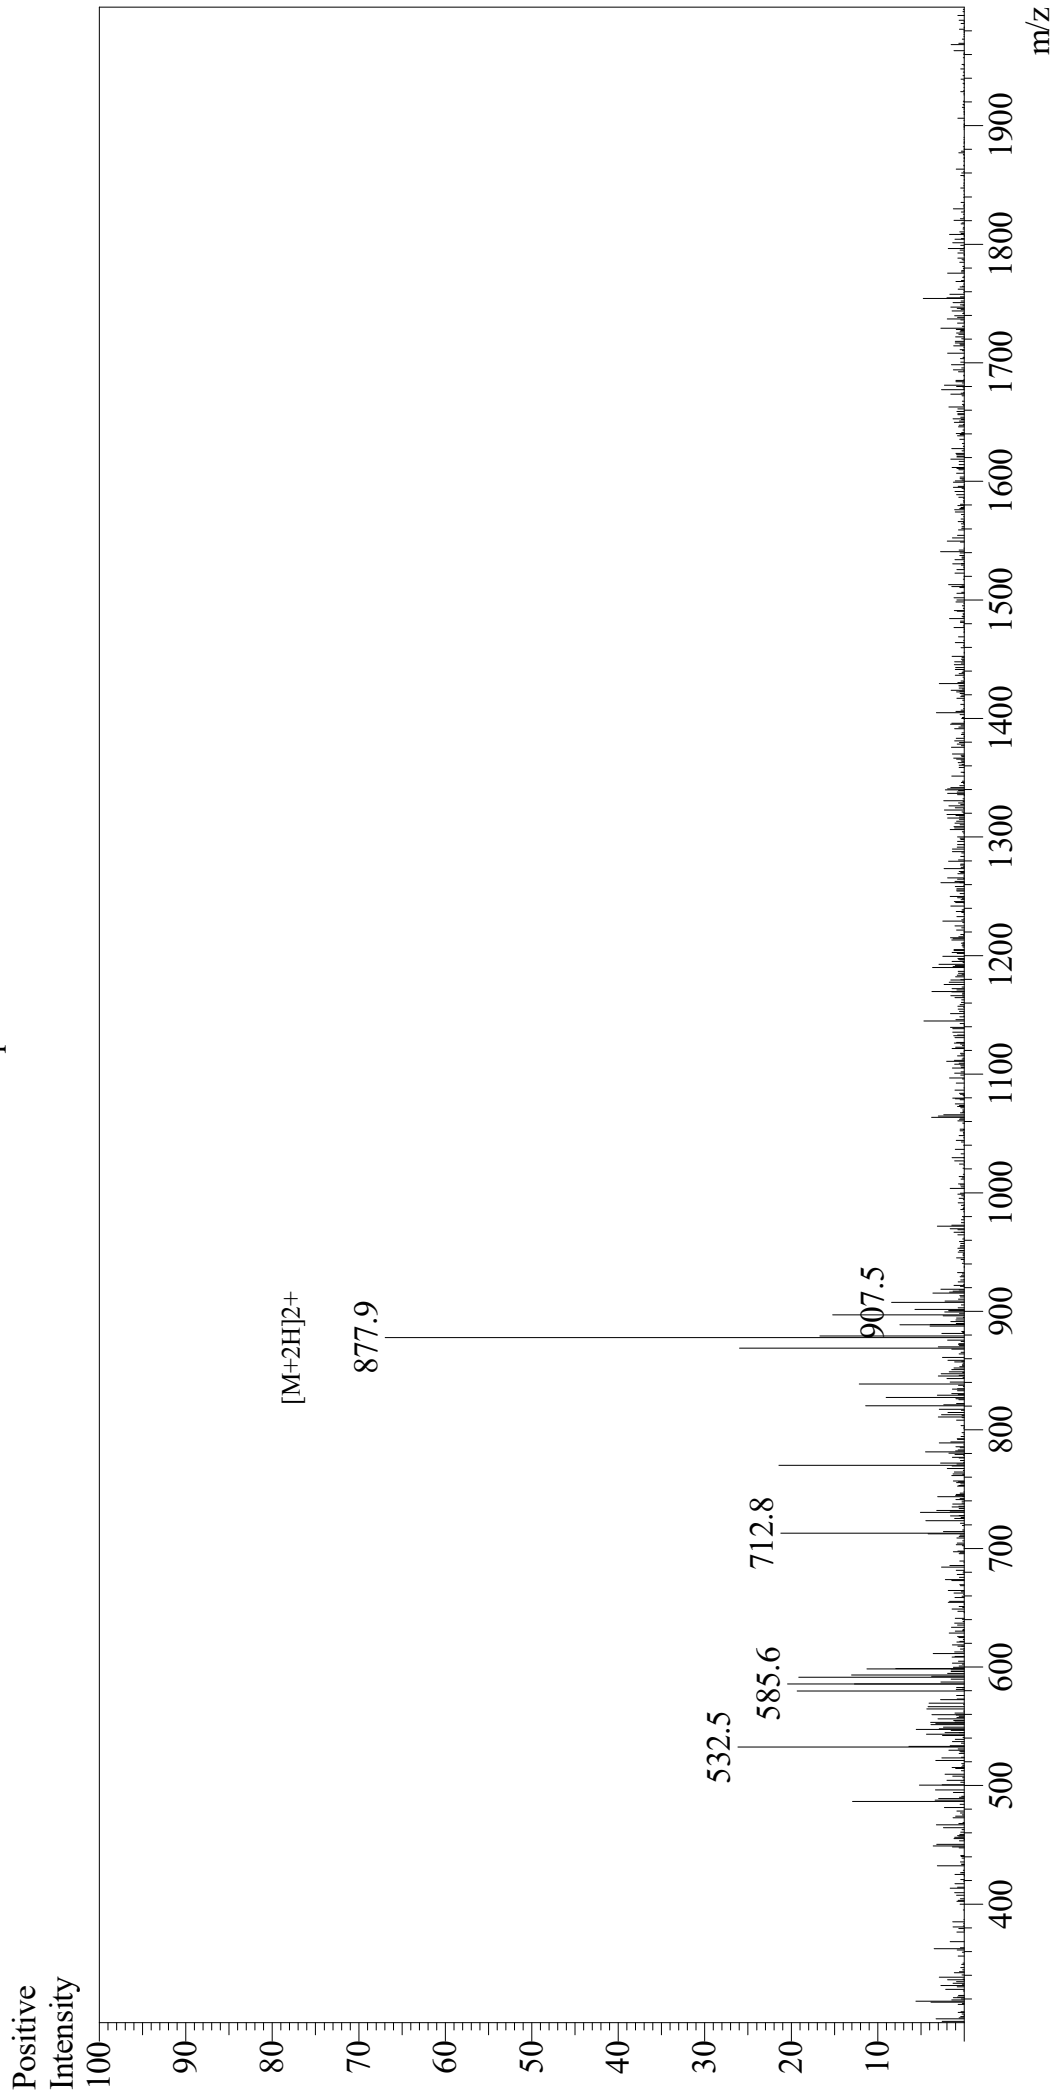

Sample Information

User : Gary
Month-Day Processed : 04/23/19
Time Processed : 11:09:05 AM
Injection Volume : 0.3
Sample Name : HEL(46-61)
Cat No. : RP11736
Lot No. : PE9641904
Theoretical MW : 1753.83
Observed MW : 1753.8

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH