

Sample Name : C-telopeptide  
 Cat. No. : RP10566  
 Lot. No. : E0771219J  
 Time Processed :10:30:17  
 Month-Day-Year Processed :10/23/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	15	
40.00	Pumps	Pump B Conc.	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

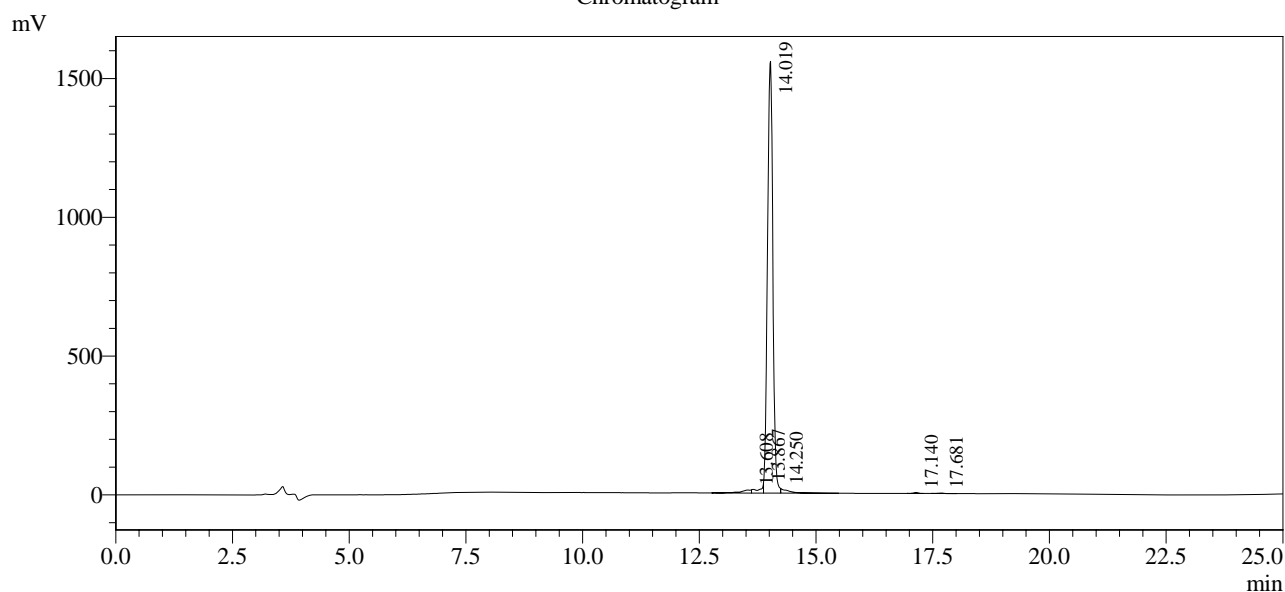

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.608	166402	10911	1.277
2	13.867	213515	25624	1.638
3	14.019	12412671	1555830	95.229
4	14.250	206702	15839	1.586
5	17.140	22722	3342	0.174
6	17.681	12517	1675	0.096
Total		13034529	1613222	100.000