


Mass Spectrum

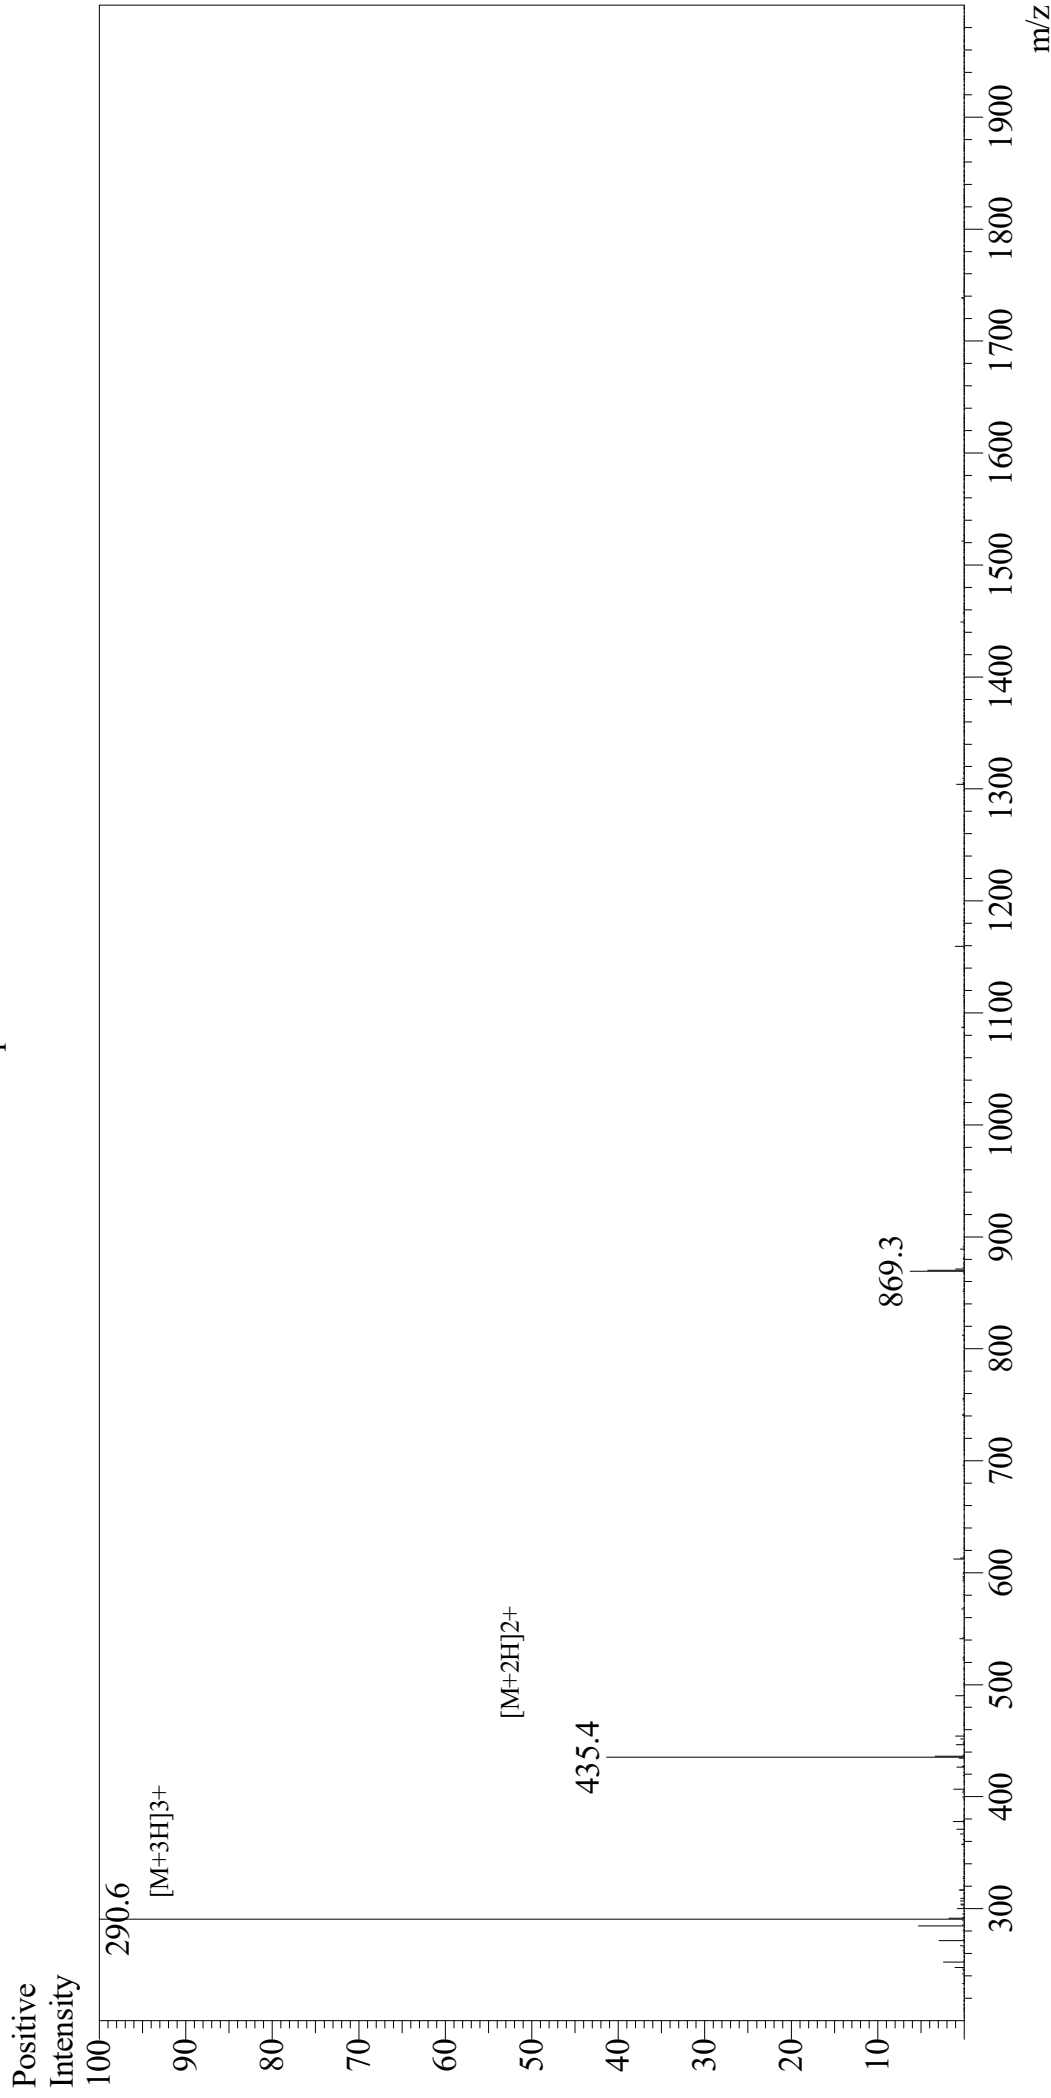

Sample Information

User : Gary

Month-Day Processed : 10/21/19

Time Processed : 02:14:53 PM

Injection Volume : 0.3

Sample Name : C-telopeptide

Cat No. : RP10566

Lot No. : E0771219J

Theoretical MW : 868.90

Observed MW : 868.8

Interface : ESI

Nebulizing Gas Flow : 1.5L/min

CDL Temp : 250

Block Temp : 200

Equipment

Interface Bias

Drying Gas Flow

T.Flow

B.conc

: GK11010007

: +4.5kV

: 5 L/min

: 0.2ml/min

: 50%H2O/50%MeOH