


Mass Spectrum

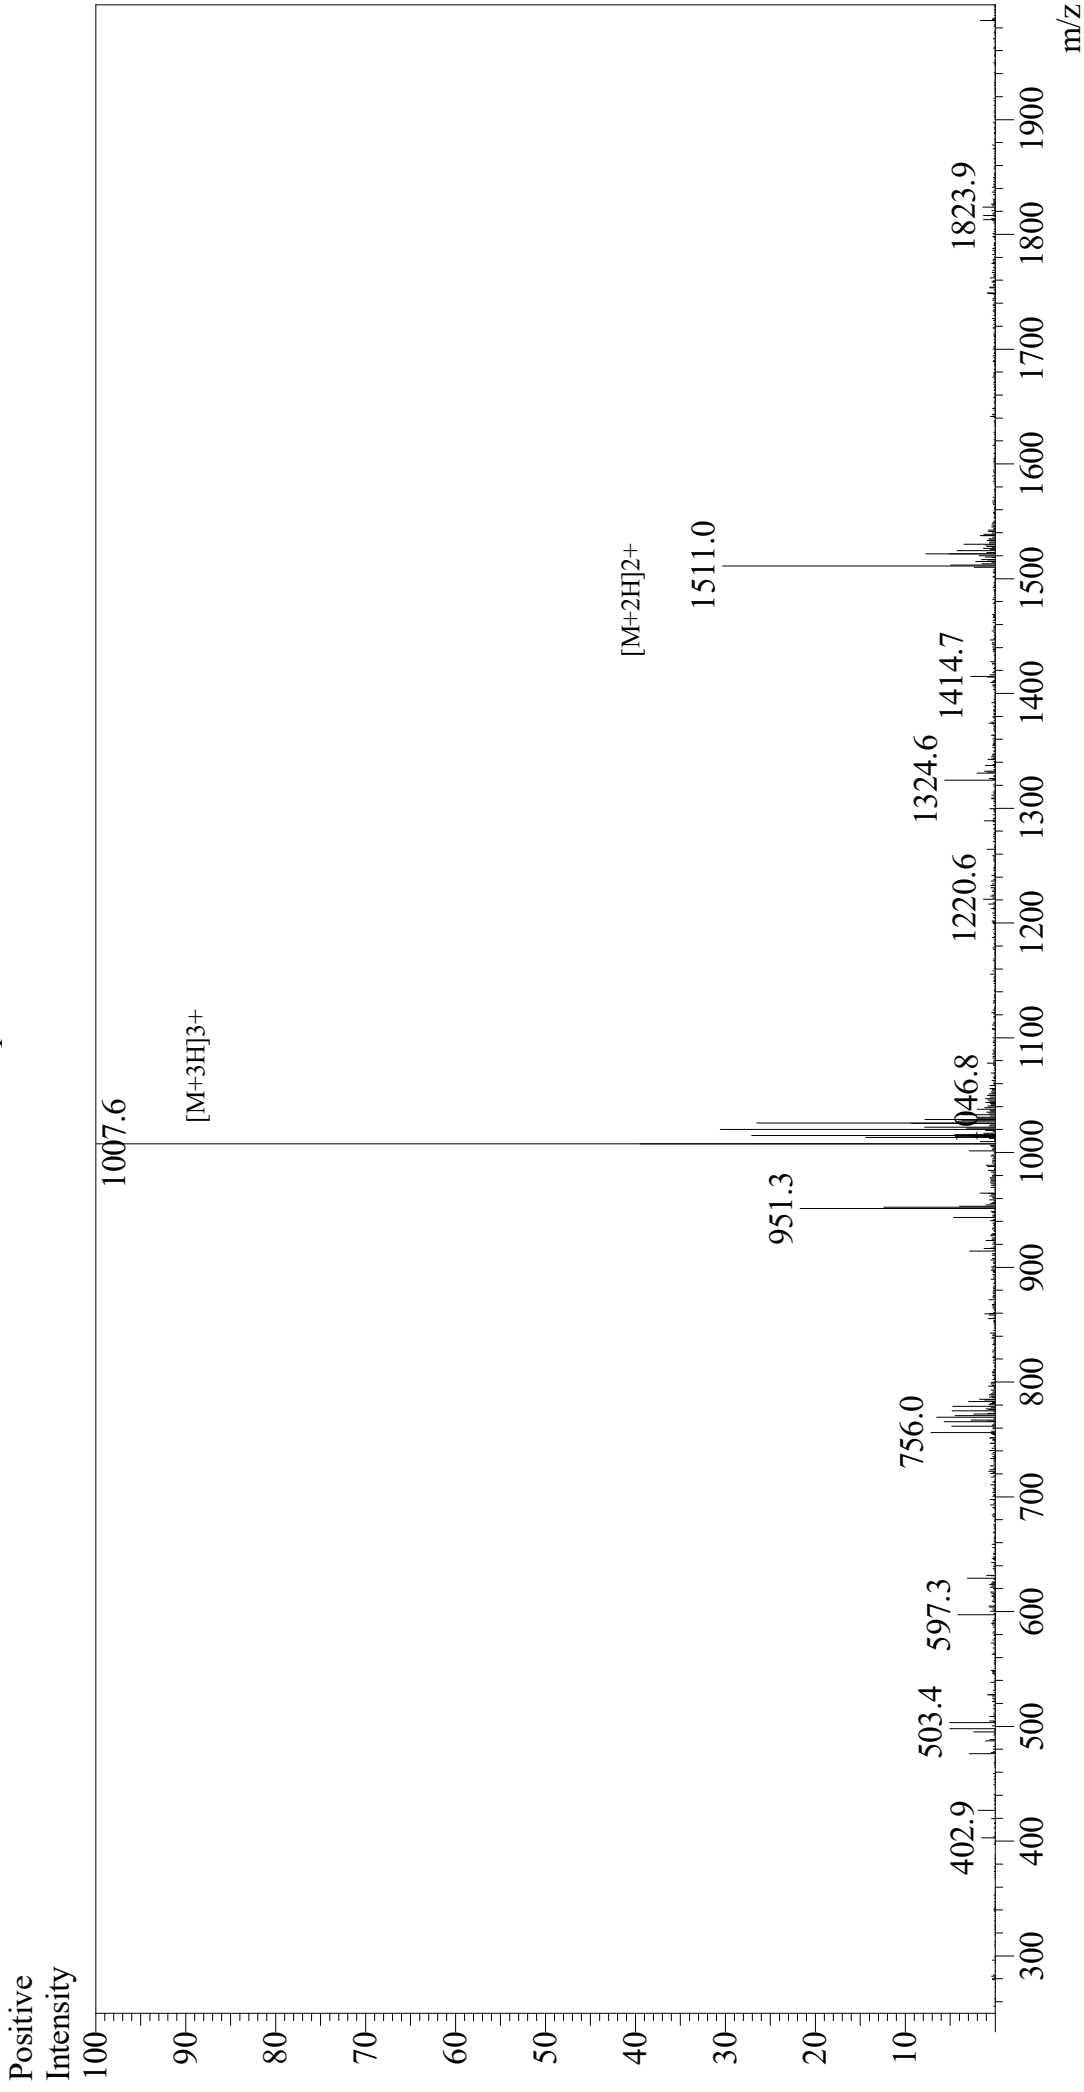

Sample Information	Equipment : GK11010007
Month-Day Processed : 12/23/20	Interface Bias : +4.5 kV
Time Processed : 4:25:39 PM	Drying Gas Flow : 5 L/min
Injection Volume : 0.3	T.Flow : 0.2 ml/min
Sample Name : C-Peptide (3-33), human	B.conc : 50% H ₂ O/50% MeOH
Cat No: RP11116	
Lot No: E8161020L	
Theoretical MW : 3020.26	
Observed MW : 3019.8	

Interface : ESI	
Nebulizing Gas Flow : 1.5 L/min	
CDL Temp : 250	
Block Temp : 200	