

Sample Name : β -Amyloid (1-15)
 Cat. No. : RP20141
 Lot. No. : PE5701704


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

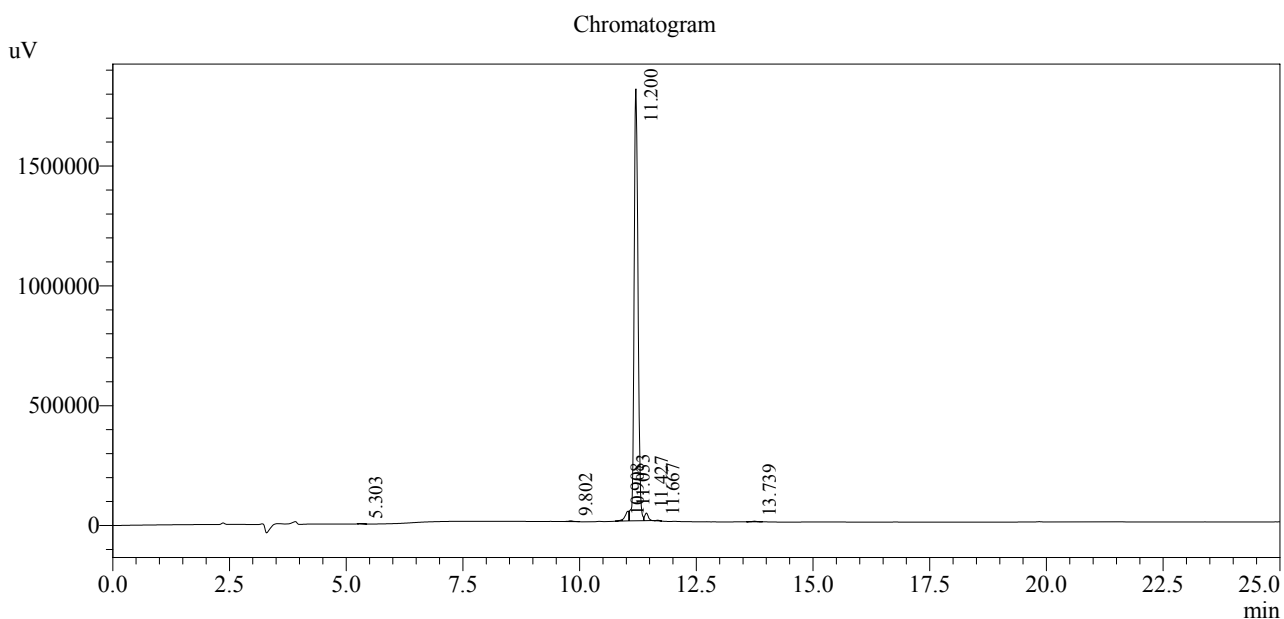

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.303	9343	1769	0.085
2	9.802	16498	2992	0.150
3	10.908	19823	4984	0.181
4	11.033	224516	40379	2.046
5	11.200	10509871	1802647	95.777
6	11.427	166698	31903	1.519
7	11.667	11246	2405	0.102
8	13.739	15266	2383	0.139
Total		10973261	1889462	100.000