

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), rat
 Cat No. : RP11090
 Lot No. : E7011319J
 Time Processed : 8:10:05 AM
 Month-Day-Year Processed : 10/02/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

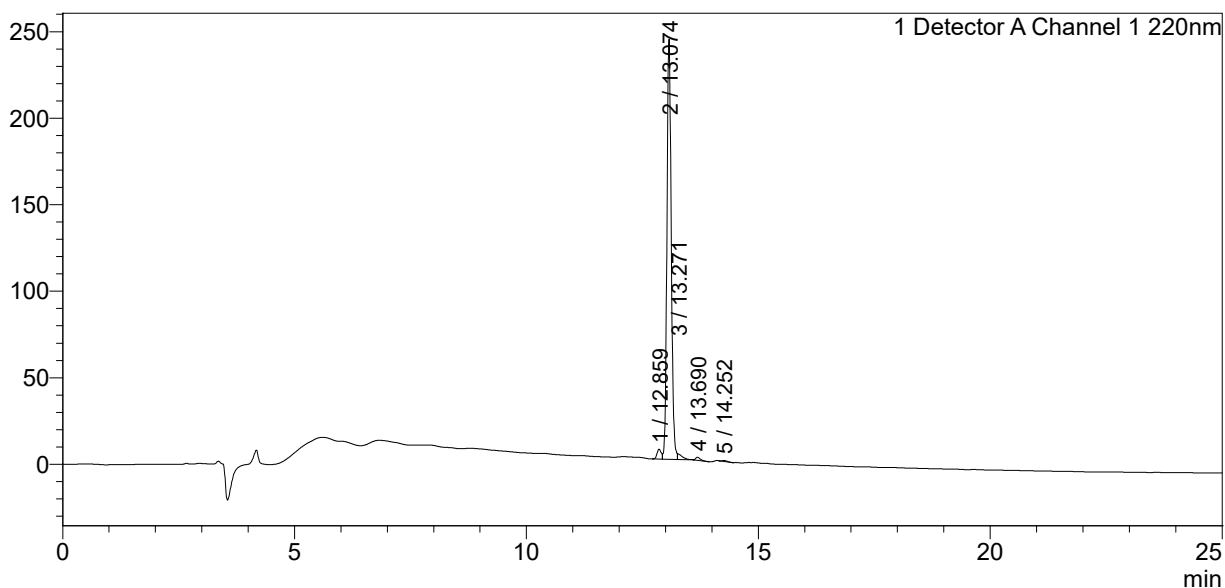

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.859	37246	5751	2.243
2	13.074	1584575	242890	95.408
3	13.271	22778	3283	1.372
4	13.690	12111	1805	0.729
5	14.252	4132	613	0.249
Total		1660843	254341	100.000