

Sample Name : -Amyloid (33-40)
 Cat No :RP20144
 Lot No :E1542720L
 Time Processed :4:20:57 AM
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

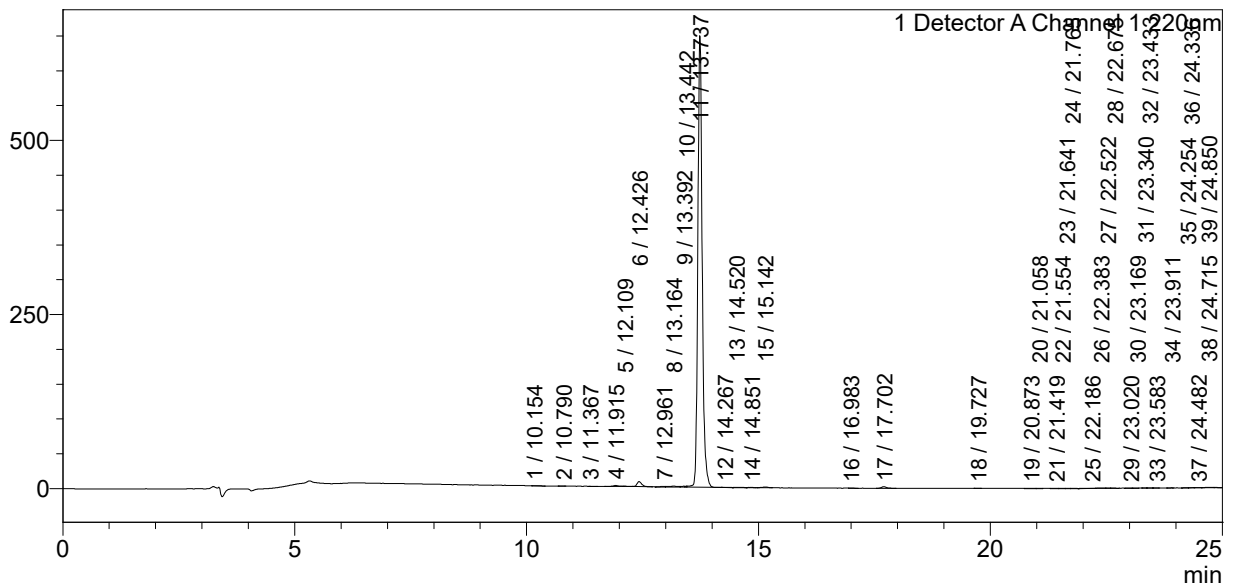

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.154	1927	309	0.043
2	10.790	1164	174	0.026
3	11.367	1113	149	0.025
4	11.915	12106	1323	0.272
5	12.109	2476	383	0.056
6	12.426	51646	7317	1.159
7	12.961	6352	829	0.143
8	13.164	19212	1235	0.431
9	13.392	7439	1328	0.167
10	13.442	3317	1347	0.074
11	13.737	4264686	648657	95.680
12	14.267	2605	288	0.058
13	14.520	4849	502	0.109
14	14.851	1810	351	0.041
15	15.142	9042	1015	0.203
16	16.983	1328	189	0.030

Peak#	Ret. Time	Area	Height	Area%
17	17.702	18663	2301	0.419
18	19.727	1258	194	0.028
19	20.873	3842	463	0.086
20	21.058	1742	246	0.039
21	21.419	1869	215	0.042
22	21.554	1435	205	0.032
23	21.641	1507	255	0.034
24	21.765	1345	231	0.030
25	22.186	4628	314	0.104
26	22.383	5767	559	0.129
27	22.522	2105	394	0.047
28	22.675	2840	402	0.064
29	23.020	1675	200	0.038
30	23.169	1320	216	0.030
31	23.340	1308	268	0.029
32	23.433	1652	251	0.037
33	23.583	1087	185	0.024
34	23.911	1012	218	0.023
35	24.254	1008	187	0.023
36	24.336	1177	223	0.026
37	24.482	1262	181	0.028
38	24.715	6382	702	0.143
39	24.850	1280	255	0.029
Total		4457239	674060	100.000