

Sample Name :β-Endorphin, human
 Cat No. :RP11344
 Lot No. :E9864121I
 Time Processed : 12:27:14
 Month-Day-Year Processed : 11/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	15
35.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

mV

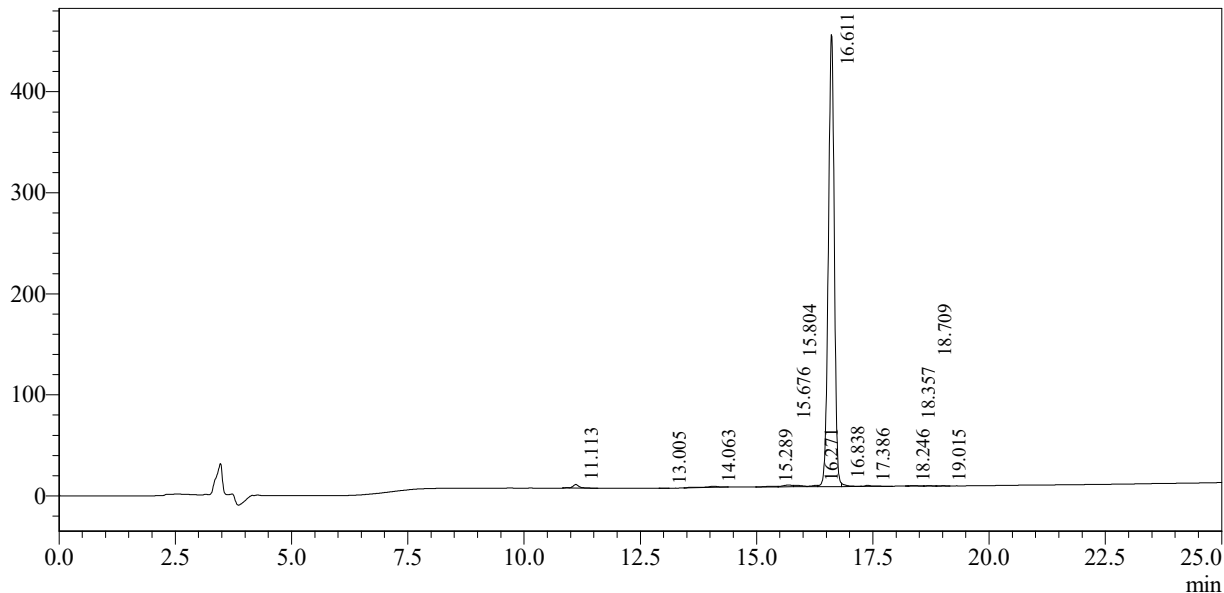

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.113	37098	3613	0.896
2	13.005	545	70	0.013
3	14.063	20842	944	0.503
4	15.289	9203	579	0.222
5	15.676	24057	1758	0.581
6	15.804	17536	1341	0.424
7	16.271	12184	1260	0.294
8	16.611	3980833	447202	96.147
9	16.838	18414	2960	0.445
10	17.386	10663	1046	0.258
11	18.246	30	16	0.001
12	18.357	5255	455	0.127
13	18.709	2657	311	0.064
14	19.015	1041	158	0.025
Total		4140359	461712	100.000