

Sample Name : PACAP (1-27), human, ovine, rat
 Cat No.: RP10334
 Lot No.: PE5091905
 Time Processed : 9:56:18
 Month-Day-Year Processed : 05/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010509

<Chromatogram>

mV

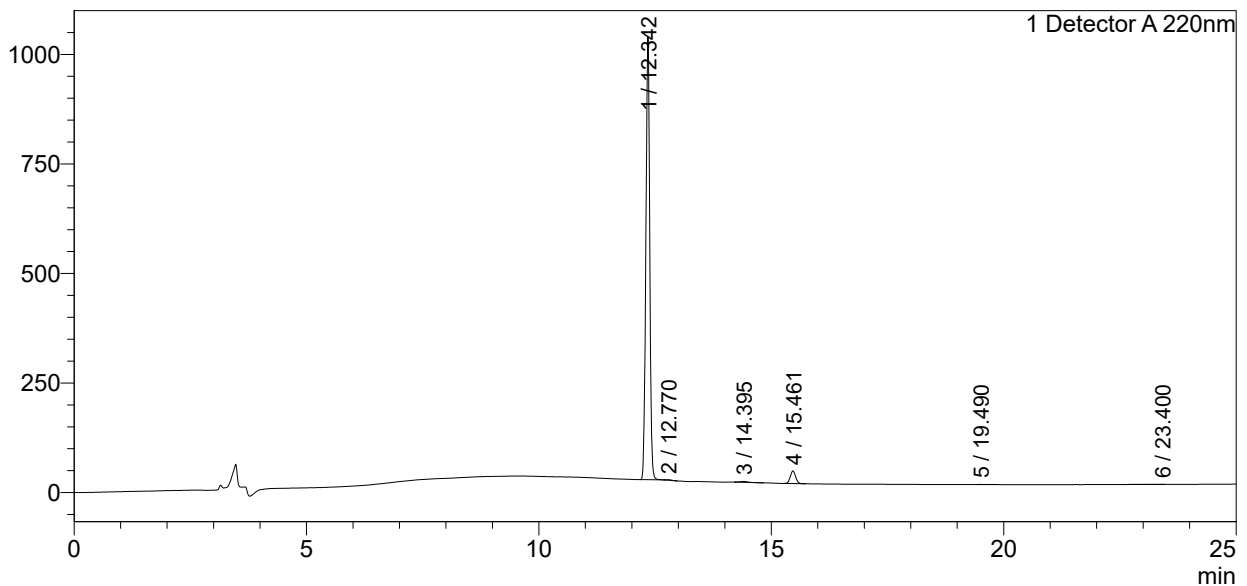

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.342	5827230	1012113	95.605
2	12.770	9988	1269	0.164
3	14.395	24583	2317	0.403
4	15.461	229542	28887	3.766
5	19.490	1577	198	0.026
6	23.400	2207	28	0.036
Total		6095126	1044812	100.000