

Sample Name :HIV gag peptide (199-207)
 Cat No. :RP20251
 Lot No. :E7055719J
 Time Processed :10:42:23 AM
 Month-Day-Year Processed :10/03/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
41.00	Pumps	Solvent B Conc.	5
41.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

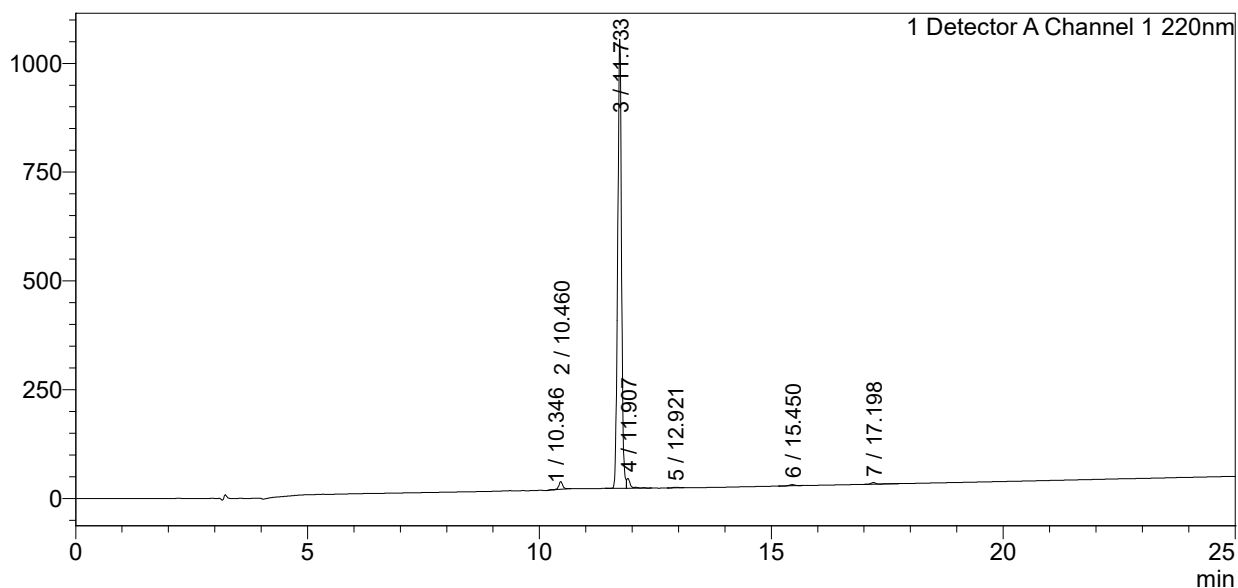

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.346	6368	484	0.102
2	10.460	103057	17778	1.653
3	11.733	5948479	1032242	95.430
4	11.907	116610	22210	1.871
5	12.921	11948	1567	0.192
6	15.450	21086	2818	0.338
7	17.198	25799	3838	0.414
Total		6233346	1080938	100.000