


Mass Spectrum

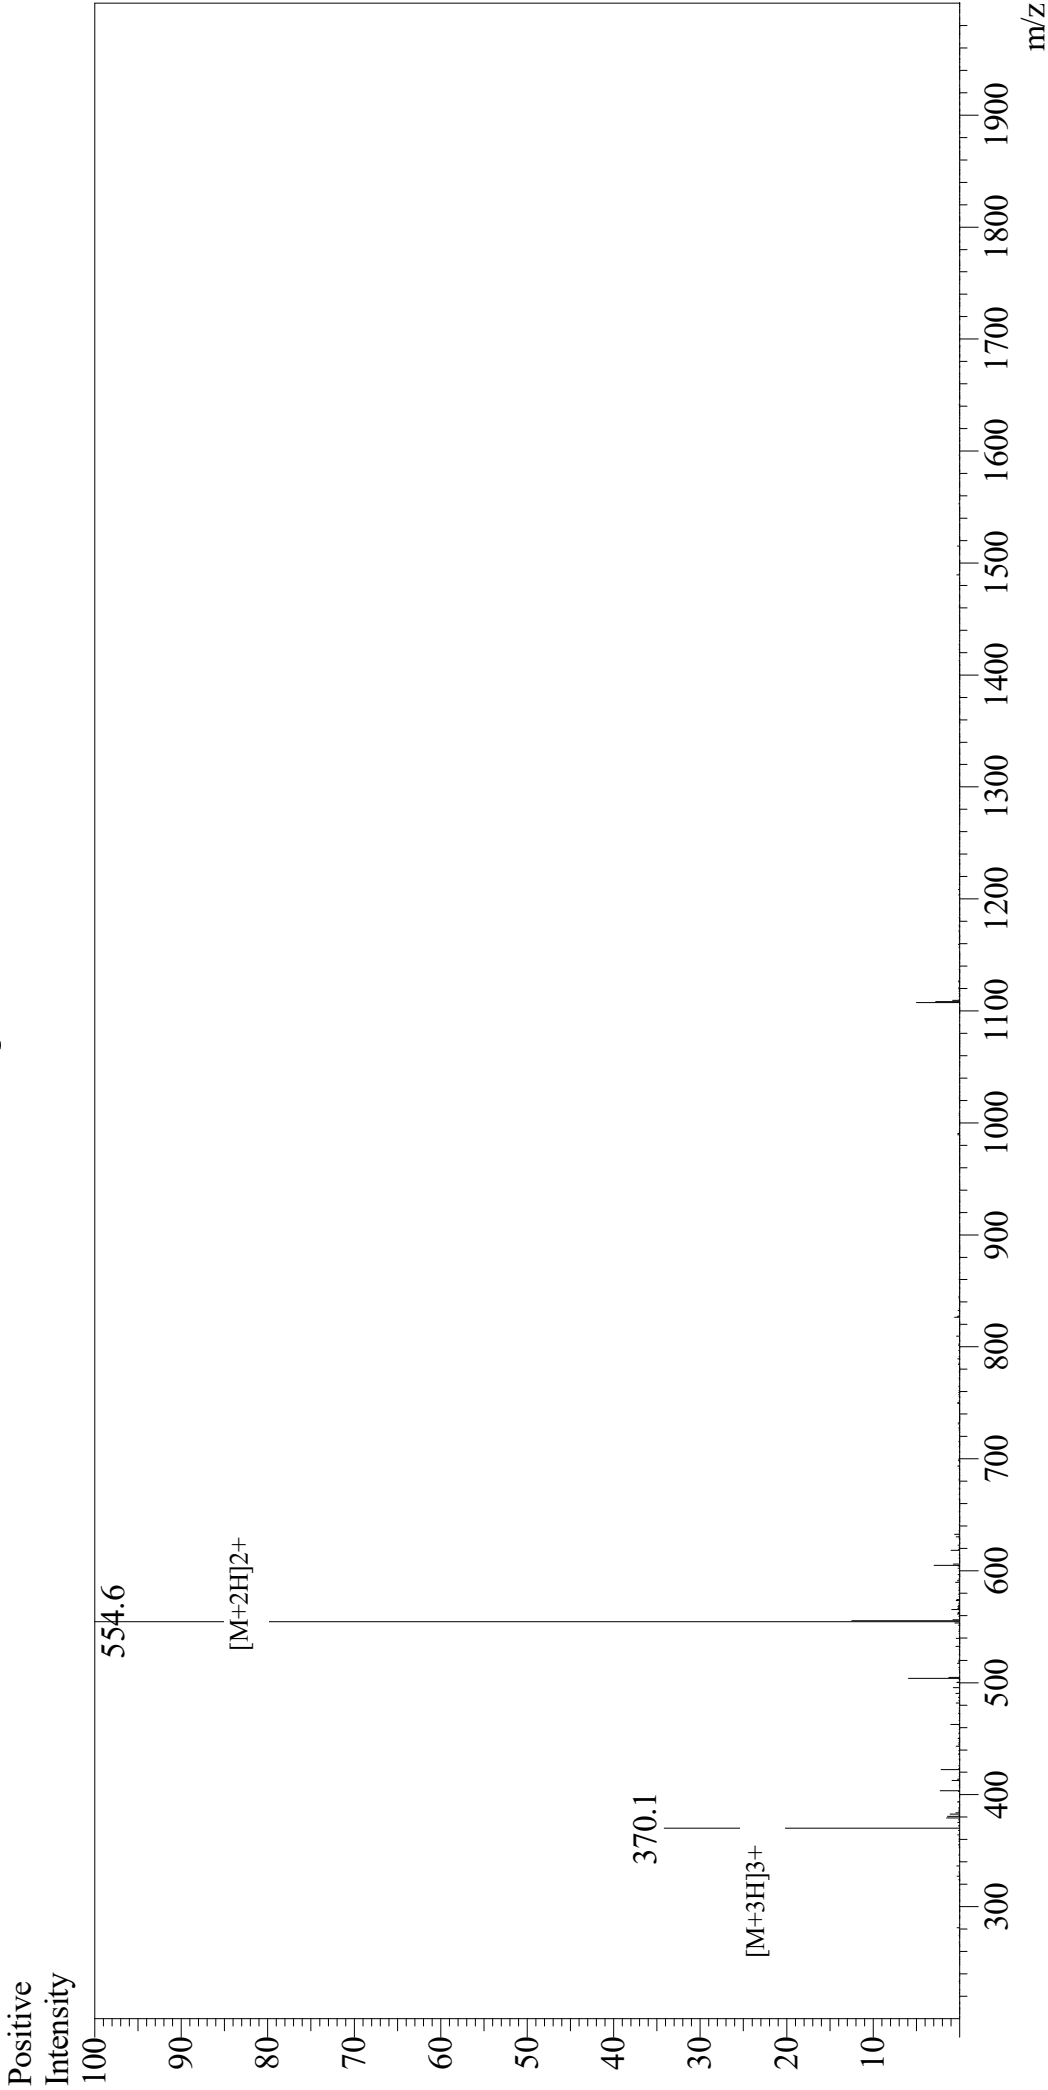

Sample Information

User :	Gary	Equipment	: GK11010007
Month-Day Processed :	03/01/19	Interface Bias	: +4.5kV
Time Processed :	02:37:31 PM	Drying Gas Flow	: 5 L/min
Injection Volume :	0.2	T.Flow	: 0.2ml/min
Sample Name :	Influenza NP (147-155)	B.conc	: 50% H ₂ O / 50% MeOH
Cat No. :	RP20260-1		
Lot No. :	PE8641902		
Theoretical MW :	1107.27		
Observed MW :	1107.2		