


Mass Spectrum

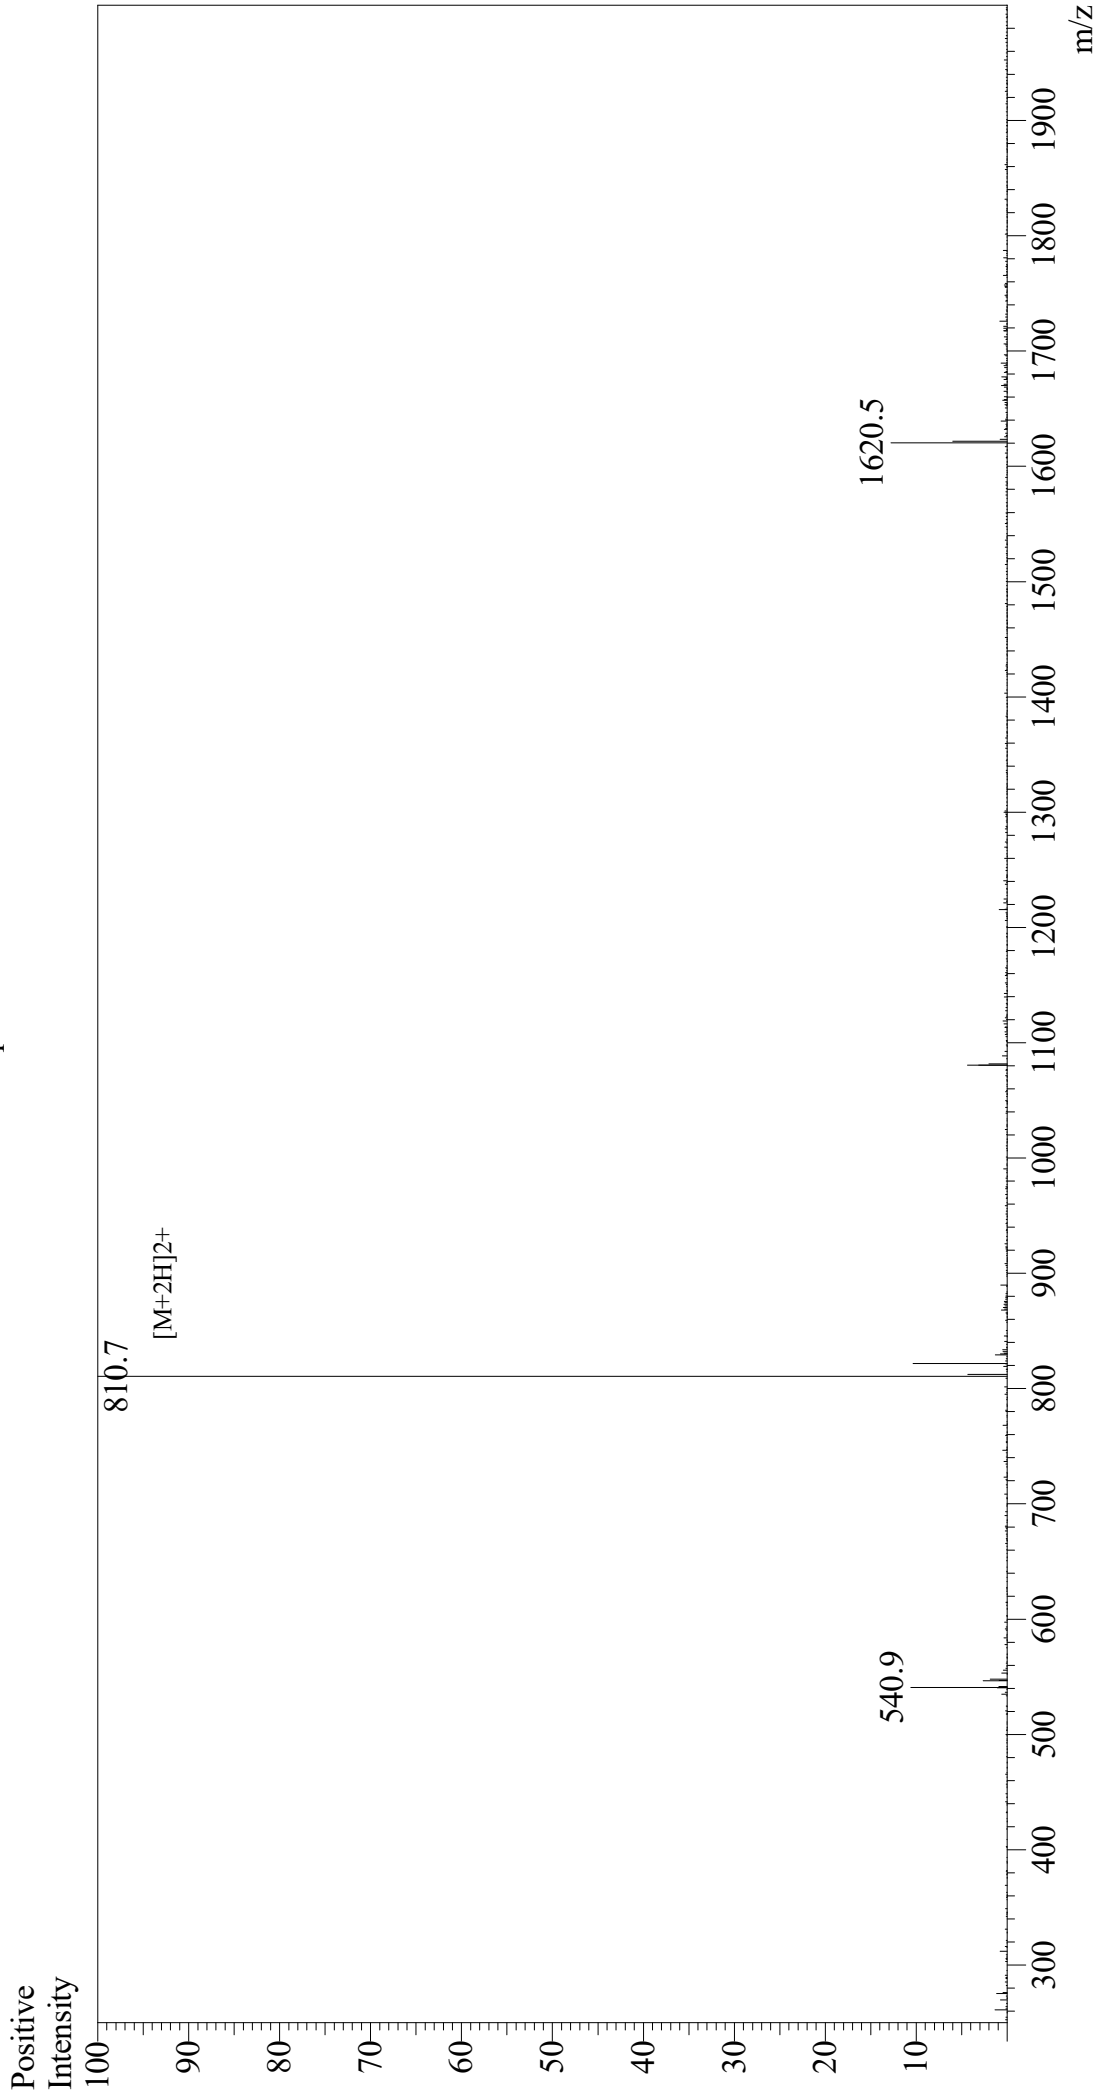

Sample Information
Month-Day Processed : 01/26/21
Time Processed : 7:11:08 PM
Injection Volume : 0.4
Sample Name : Bombesin
Cat No. : RP111157
Lot No. : E0675021A
Theoretical MW : 1619.90
Observed MW : 1619.4

Interface : ESI
Nebulizing Gas Flow : 1.5 L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O/50% MeOH