


Mass Spectrum

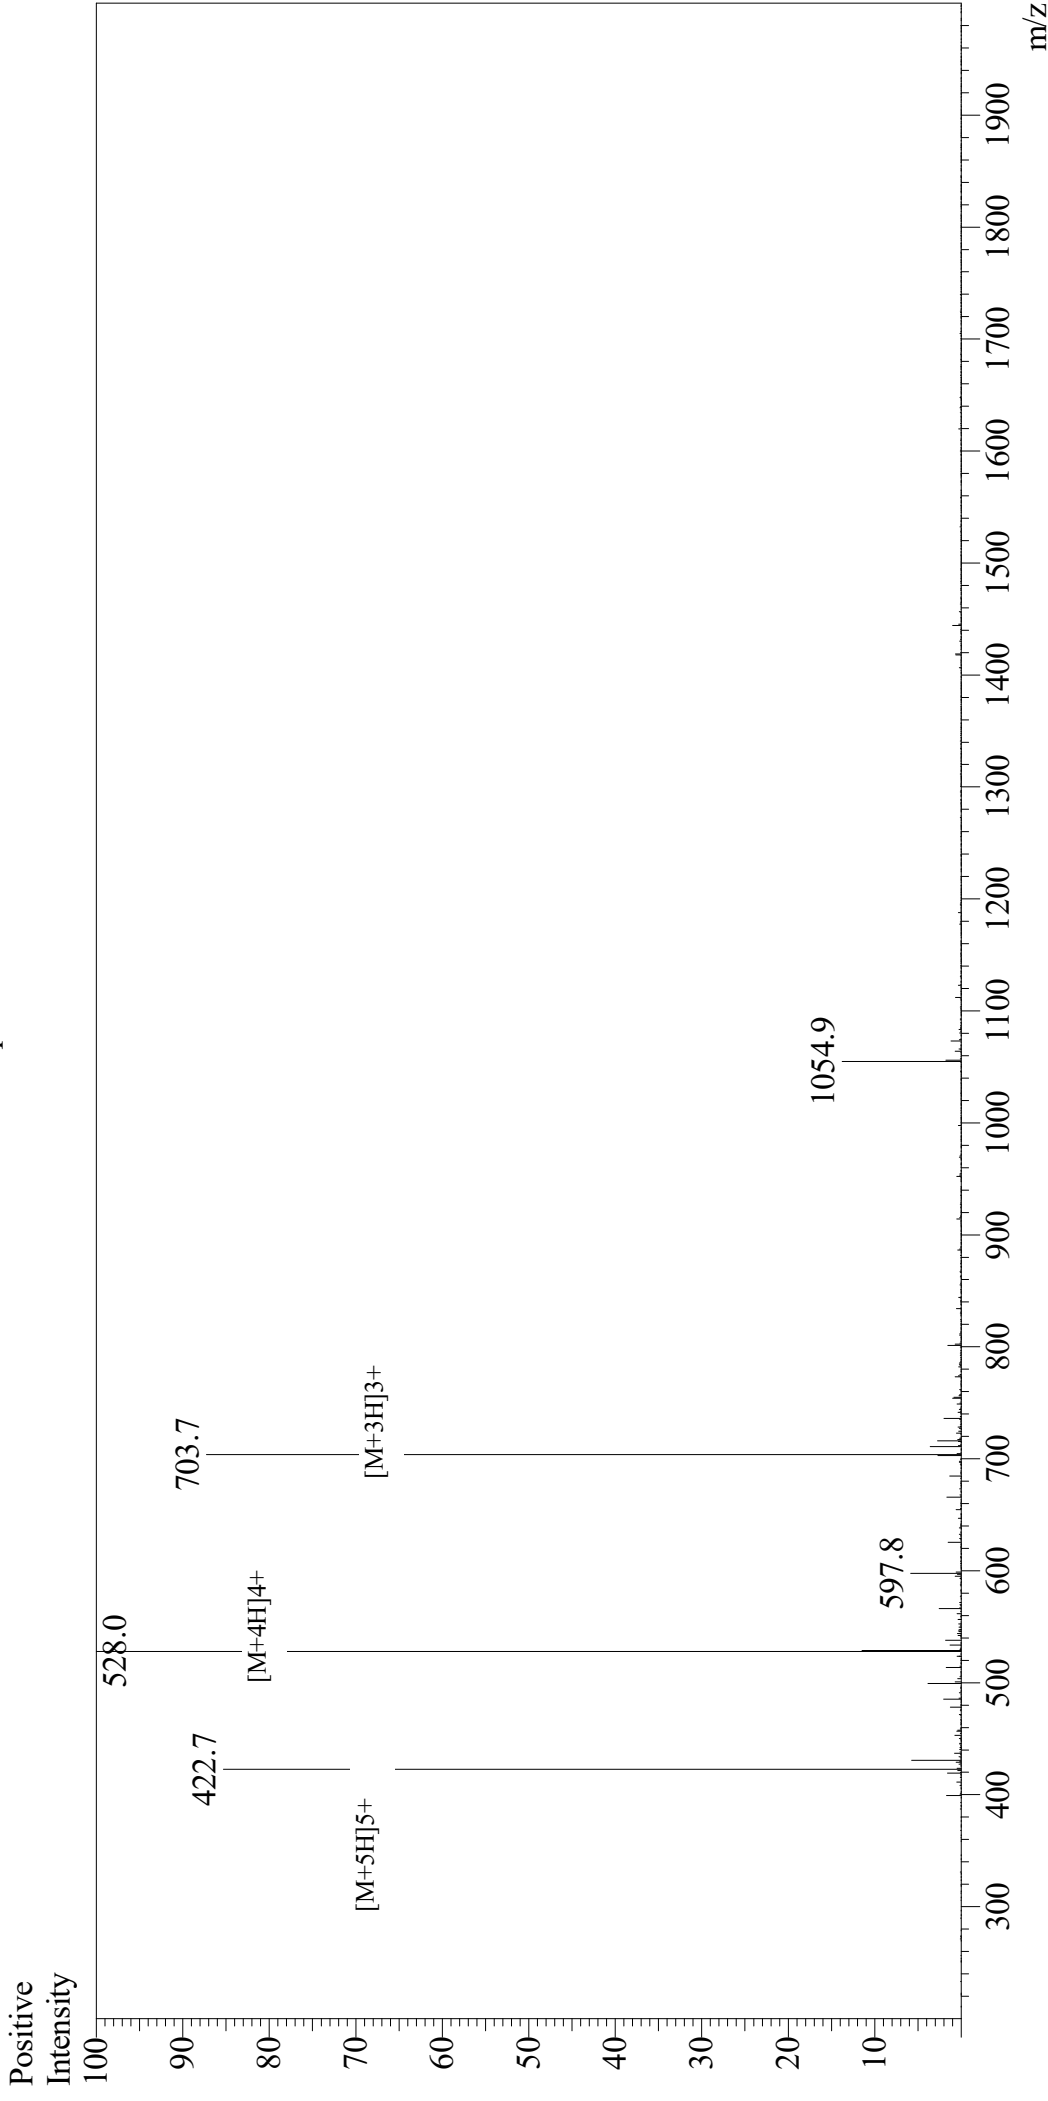

Sample Information

User : Gary
Month-Day Processed : 03/04/19
Time Processed : 05:11:00 PM
Injection Volume : 0.2
Sample Name : Apidaecin IB
Cat No. : RP20409
Lot No. : PE9001902
Theoretical MW : 2108.40
Observed MW : 2108.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH