

Sample Name :Neurotensin  
 Cat No. : RP10439  
 Lot No. : E3873201  
 Time Processed :1:10:22  
 Month-Day-Year Processed :09/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

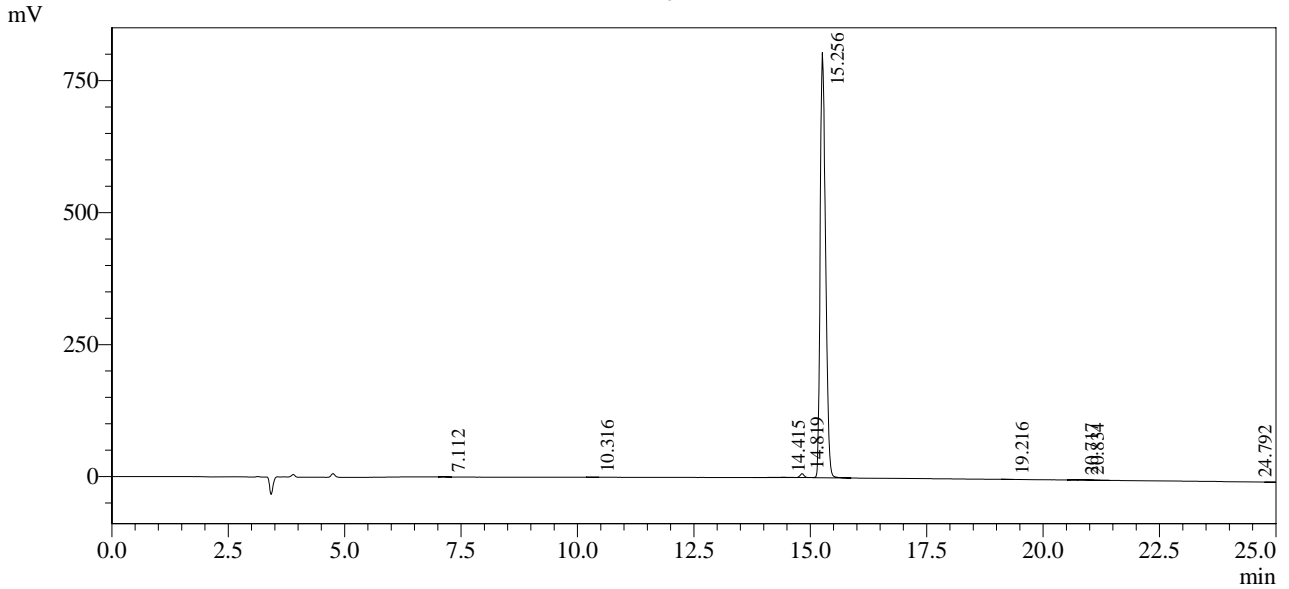

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	7.112	2313	298	0.035
2	10.316	1091	155	0.017
3	14.415	17306	633	0.264
4	14.819	45469	7380	0.694
5	15.256	6460264	804968	98.588
6	19.216	1985	287	0.030
7	20.717	5639	678	0.086
8	20.834	17620	859	0.269
9	24.792	1083	197	0.017
Total		6552770	815456	100.000