

Sample Name :Uty HY Peptide (246-254)
 Cat No. :RP20261
 Lot No. :E2249119L
 Time Processed :20:48:34
 Month-Day-Year Processed :12/16/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

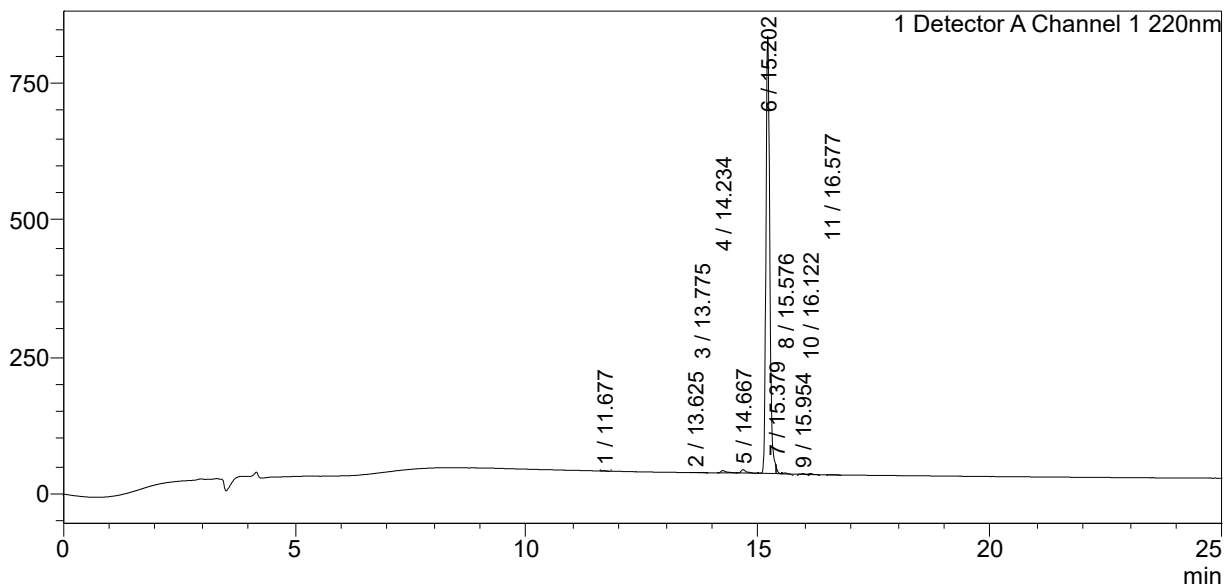

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.677	3839	722	0.081
2	13.625	1729	312	0.037
3	13.775	1861	360	0.039
4	14.234	38436	4479	0.814
5	14.667	48530	6306	1.028
6	15.202	4565351	798892	96.681
7	15.379	32230	14784	0.683
8	15.576	8656	1697	0.183
9	15.954	7894	1375	0.167
10	16.122	10840	1906	0.230
11	16.577	2725	395	0.058
Total		4722090	831228	100.000