

Sample Name :TAT peptide
 Cat No.: RP20256
 Lot No.:E2352120A
 Time Processed :20:05:15
 Month-Day-Year Processed :01/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	75
25.01	Pumps	Solvent B Conc.	95
35.00	Pumps	Solvent B Conc.	95
35.01	Pumps	Solvent B Conc.	15
40.00	Pumps	Solvent B Conc.	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

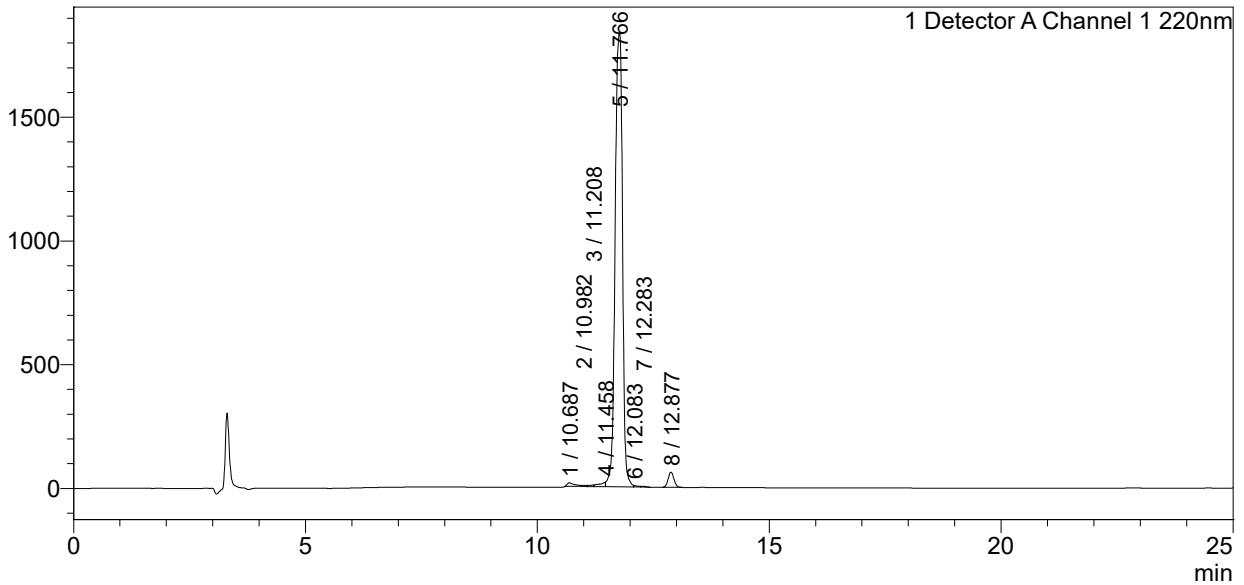

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.687	160632	13788	0.759
2	10.982	40035	5000	0.189
3	11.208	43349	6281	0.205
4	11.458	165369	17255	0.781
5	11.766	20177992	1834759	95.289
6	12.083	35391	6153	0.167
7	12.283	21904	3037	0.103
8	12.877	531006	61551	2.508
Total		21175678	1947824	100.000