


Mass Spectrum

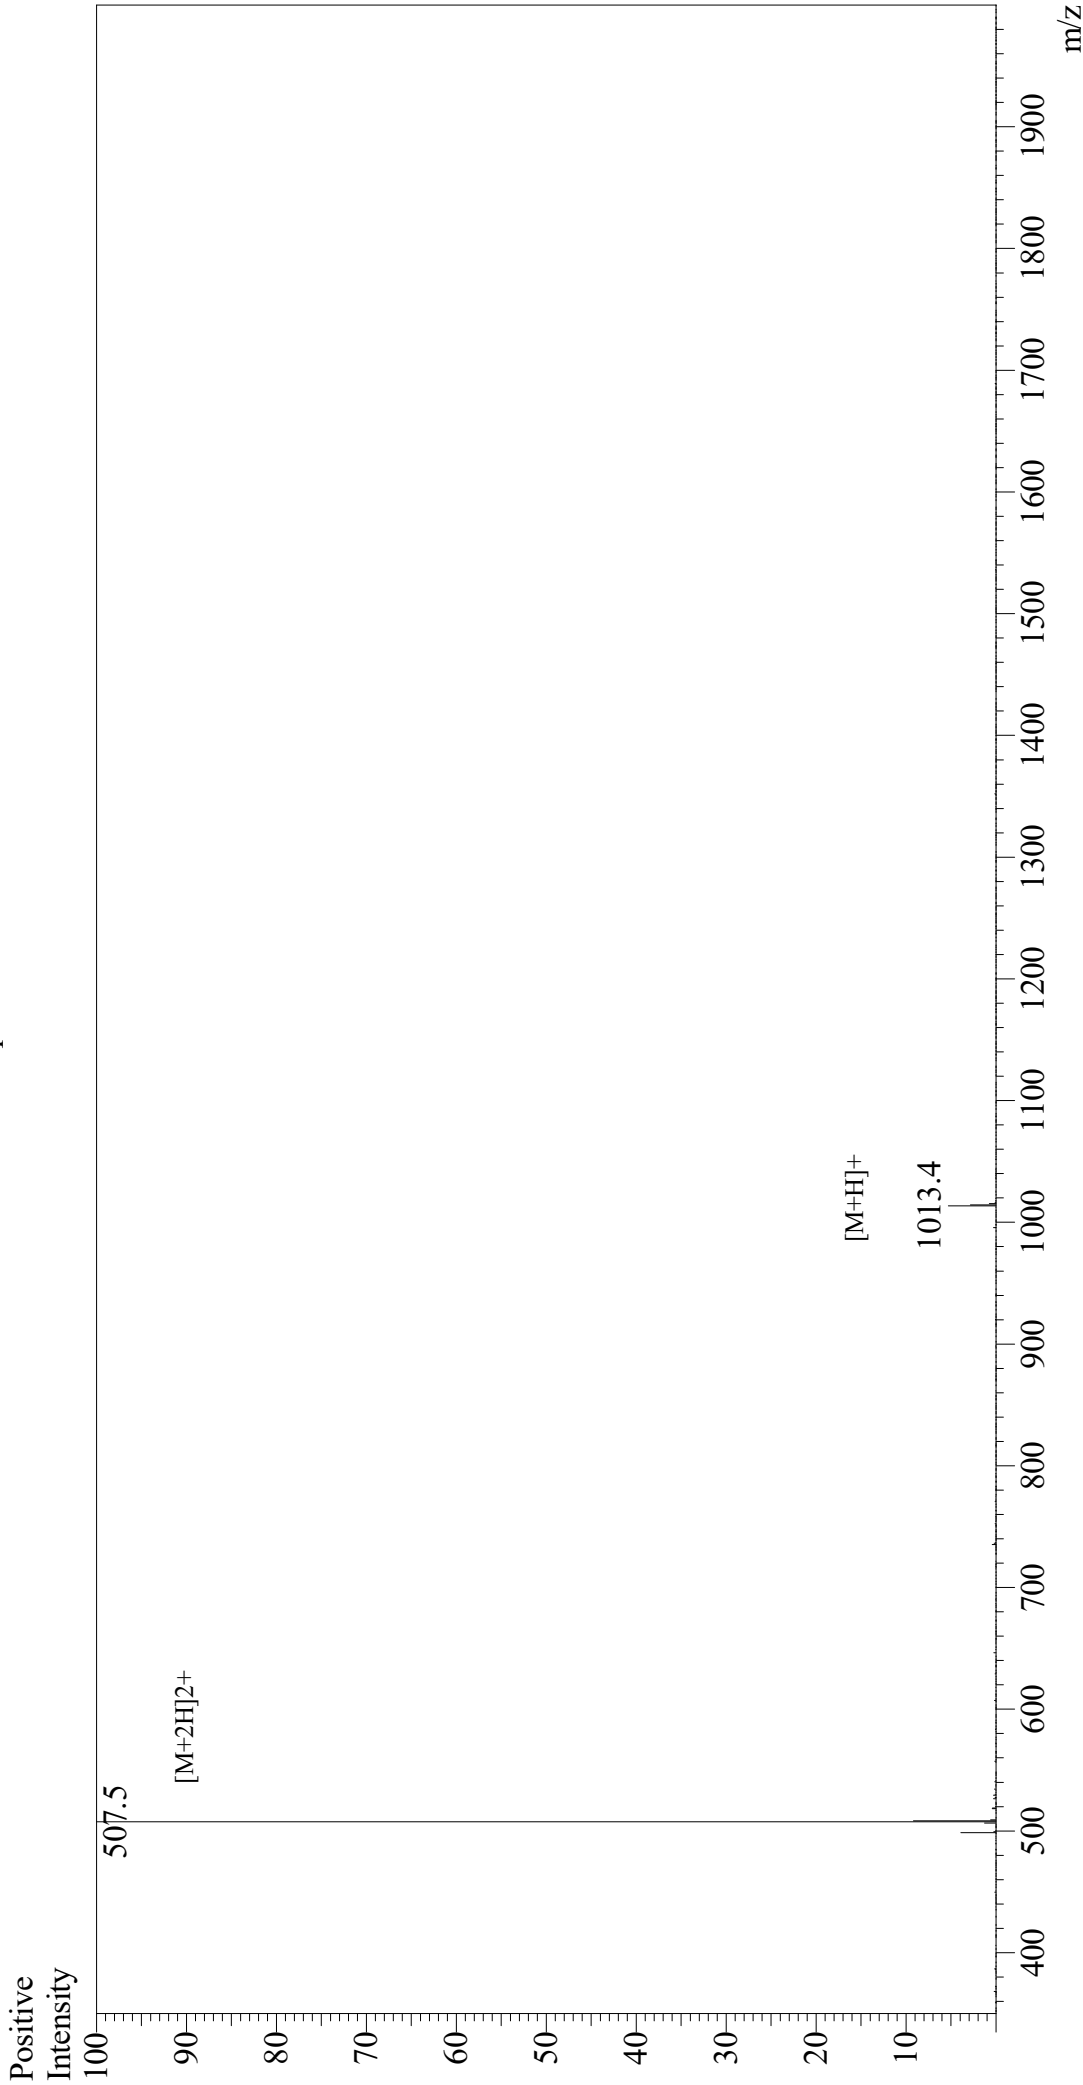

Sample Information

Month-Day Processed :	09/05/21	Equipment	: ZJ21010035
Time Processed :	20:06:55	Interface Bias	: +4.5 kV
Injection Volume :	0.2	Drying Gas Flow	: 5 L/min
Sample Name :	DYKDDDDK Peptide	T.Flow	: 0.2 ml/min
Cat No. :	RP10586	B.conc	: 50%H2O/50%MeOH
Lot No. :	E2596921H		
Theoretical MW :	1012.97		
Observed MW :	1013.0		