

Sample Name : $\beta$ -Amyloid (15-21)  
 Cat No. :RP20171  
 Lot No. :E4841719I  
 Time Processed :14:16:35  
 Month-Day-Year Processed :09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

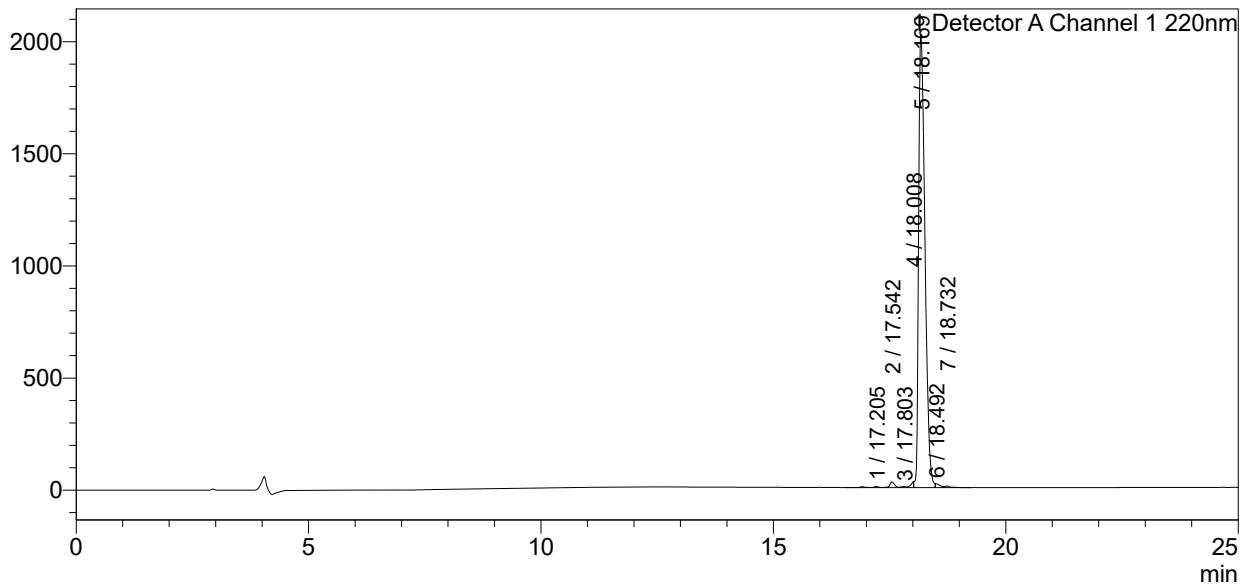

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.205	60421	5570	0.307
2	17.542	180553	25183	0.917
3	17.803	30076	4825	0.153
4	18.008	108596	26657	0.552
5	18.169	19140831	2020004	97.220
6	18.492	110814	16962	0.563
7	18.732	56820	7178	0.289
Total		19688112	2106379	100.000