

Sample Name: β -Endorphin, human
 Cat. No. : RP11344
 Lot. No. : E6670321G
 Time Processed : 8:08:01 AM
 Month-Day-Year Processed : 07/15/2021
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment : ZJ19010140

<Chromatogram>

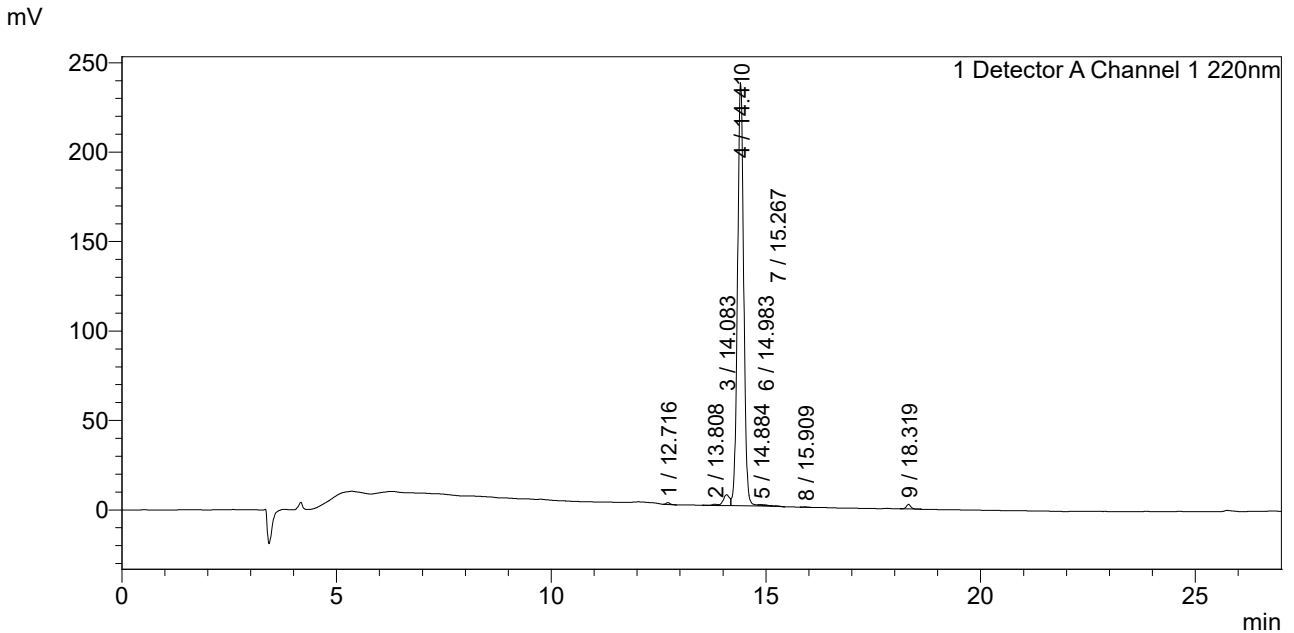

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.716	6643	1076	0.270
2	13.808	6700	738	0.272
3	14.083	62492	6119	2.536
4	14.410	2362013	236600	95.866
5	14.884	2437	436	0.099
6	14.983	1830	317	0.074
7	15.267	1287	186	0.052
8	15.909	1658	259	0.067
9	18.319	18809	2574	0.763
Total		2463869	248306	100.000