

Sample Name :PACAP (1-27), human, ovine, rat
 Cat. No. : RP10334-0.5
 Lot. No. : PE6161708

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

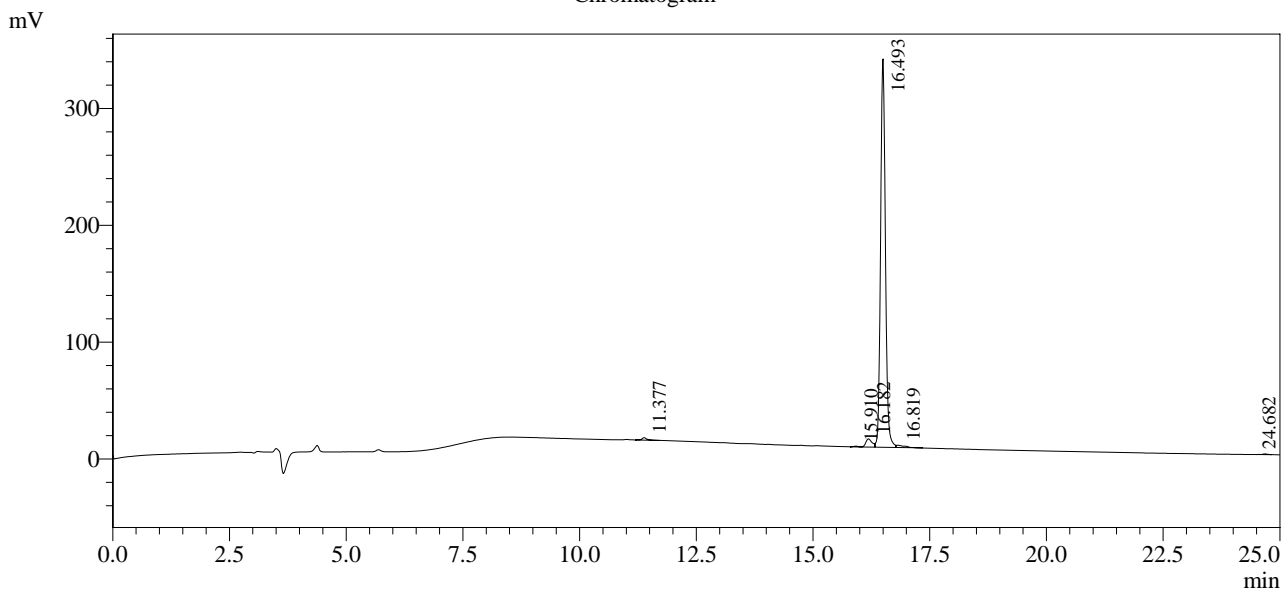

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.377	16382	2083	0.650
2	15.910	4431	666	0.176
3	16.182	66042	7091	2.622
4	16.493	2402873	332525	95.405
5	16.819	24730	1900	0.982
6	24.682	4136	569	0.164
Total		2518594	344833	100.000