

Sample Name :Influenza HA (518-526)  
 Cat No. :RP20284  
 Lot No. :E7536819K  
 Time Processed :7:49:04  
 Month-Day-Year Processed :11/09/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

### <Chromatogram>

mV

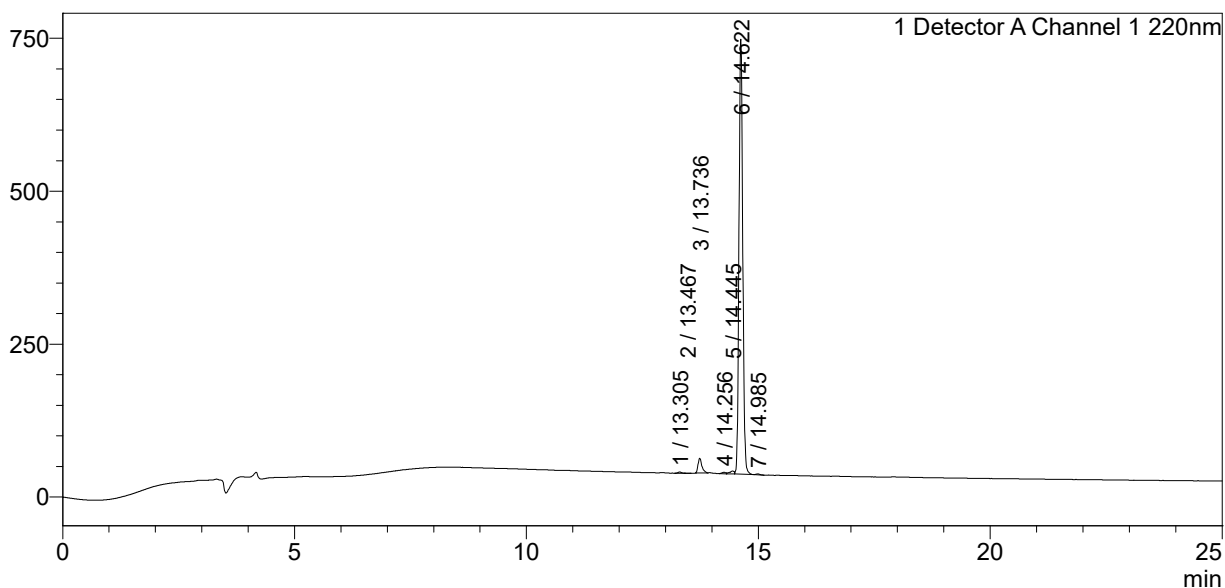

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.305	10131	1850	0.239
2	13.467	1147	216	0.027
3	13.736	137082	23803	3.237
4	14.256	12464	2210	0.294
5	14.445	32894	4801	0.777
6	14.622	4033974	711613	95.246
7	14.985	7641	1519	0.180
Total		4235332	746012	100.000