

Sample Name : Ghrelin, rat
 Cat. No. : RP10781
 Lot. No. : PE7891812
 Time Processed : 17:52:23
 Month-Day-Year Processed : 12/21/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

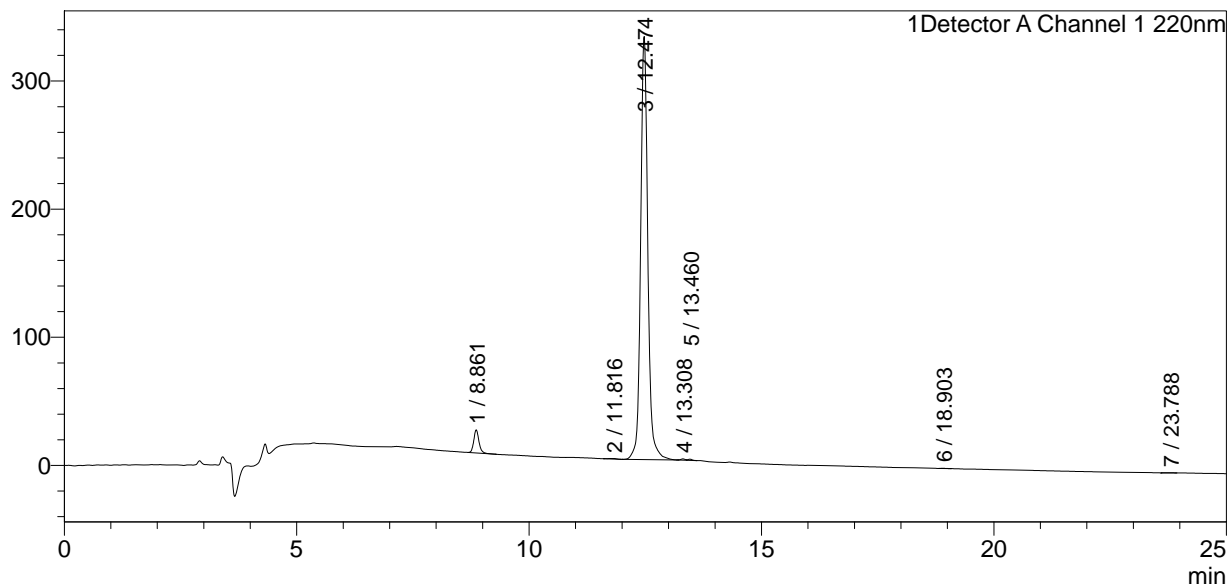

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.861	139997	18046	3.792
2	11.816	4997	479	0.135
3	12.474	3533371	330203	95.708
4	13.308	5871	941	0.159
5	13.460	5244	891	0.142
6	18.903	1072	138	0.029
7	23.788	1283	125	0.035
Total		3691834	350823	100.000