

Sample Name : Cortistatin 14, human, rat
 Cat. No. : RP10972
 Lot. No. : PE6071702

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

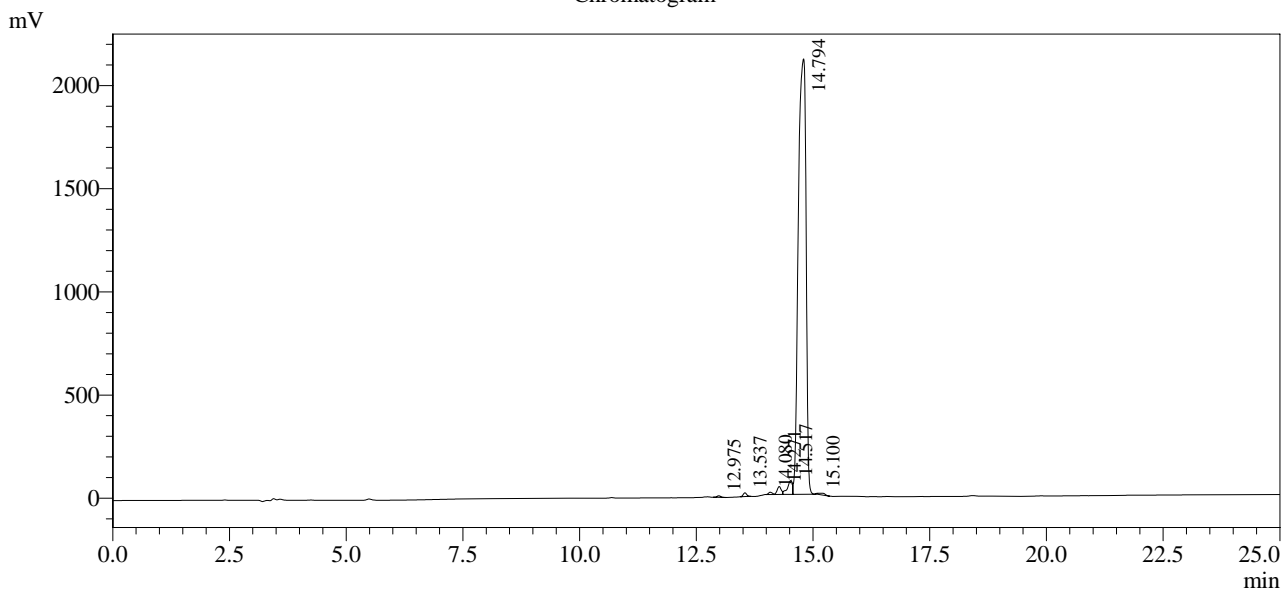

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.975	41983	7735	0.166
2	13.537	91591	17909	0.363
3	14.080	64423	11257	0.255
4	14.271	233679	38187	0.926
5	14.517	504266	66855	1.999
6	14.794	24210515	2110180	95.955
7	15.100	84664	5031	0.336
Total		25231121	2257155	100.000