


Mass Spectrum

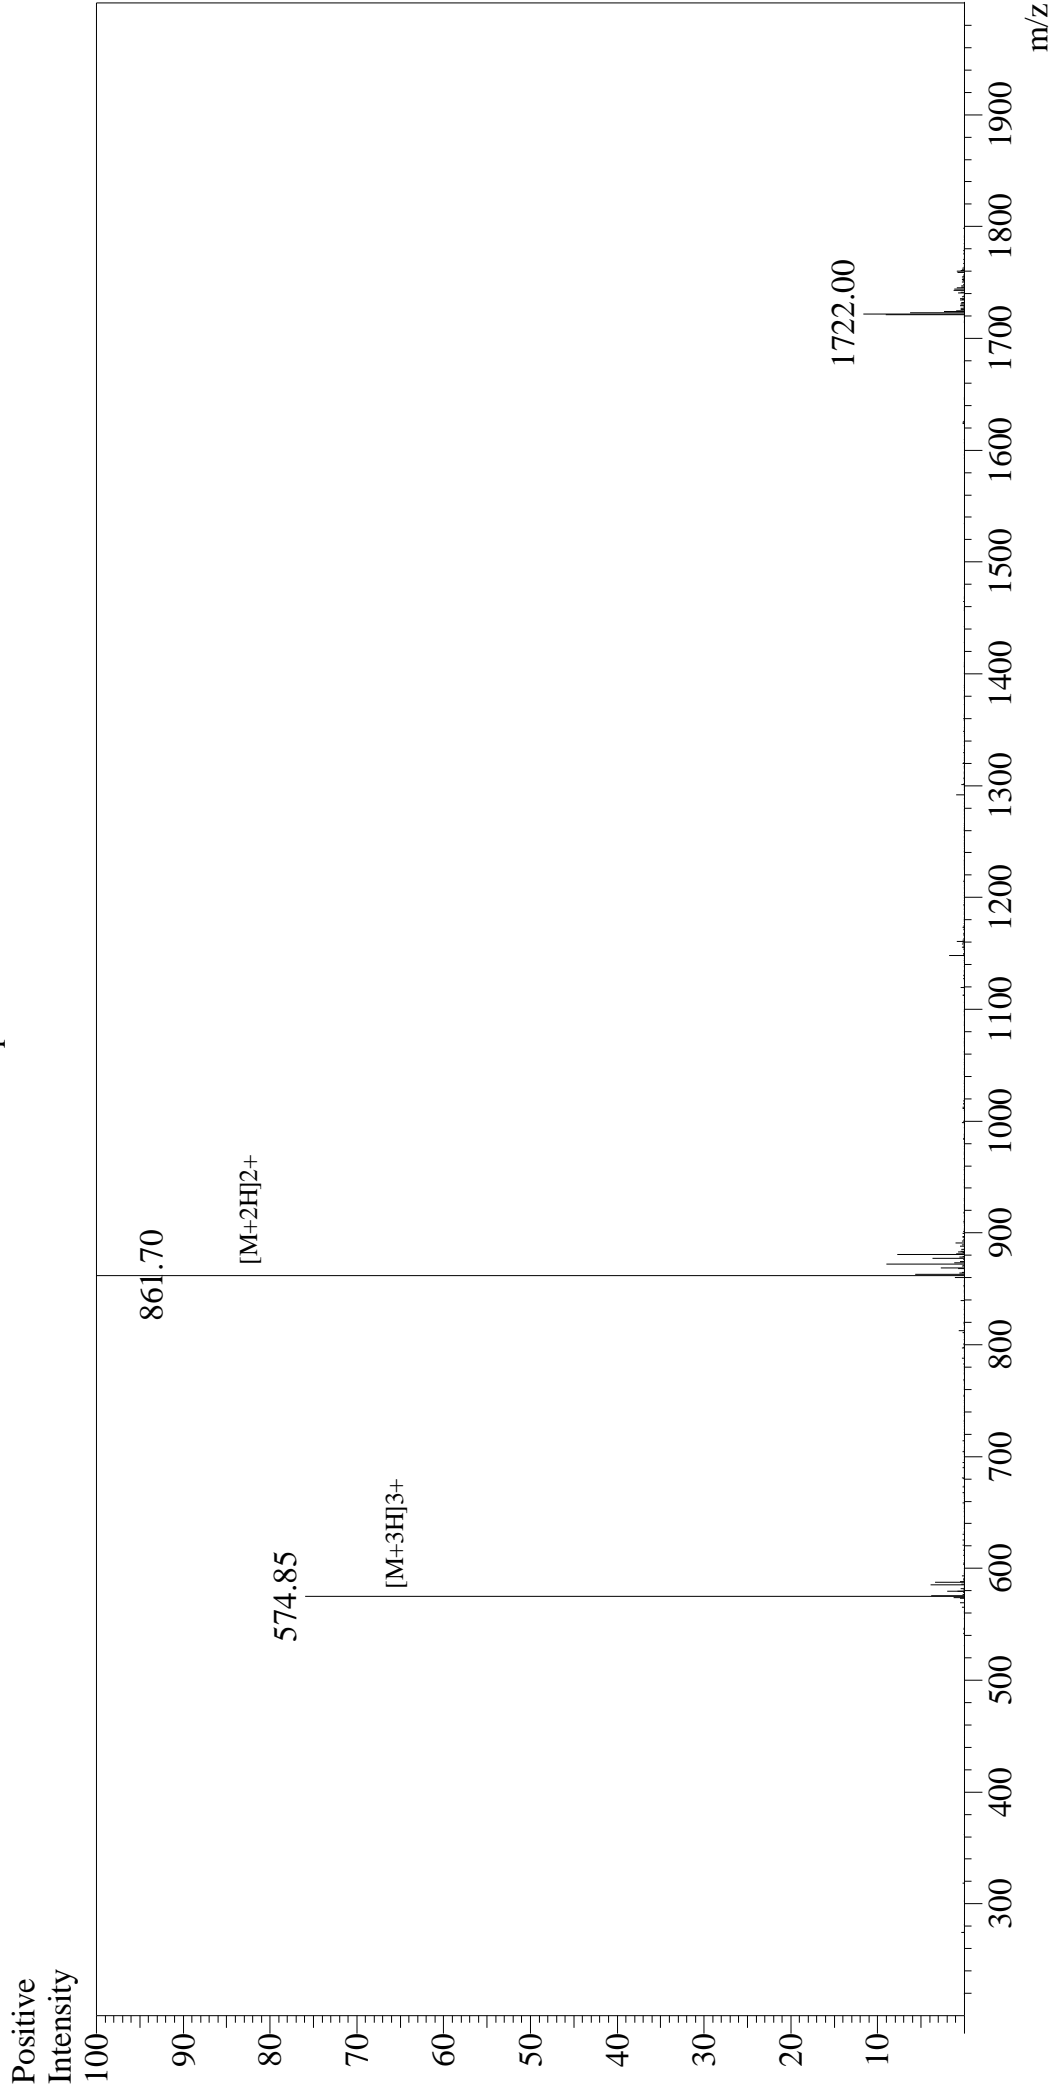

Sample Information

User : Gary
Month-Day Processed : 02/21/17
Time Processed : 10:02:38
Injection Volume : 0.2
Sample Name : Cortistatin 14, human, rat
Cat No. : RPI0972
Lot No. : PE6071702
Theoretical MW : 1721.01
Observed MW : 1721.40

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH