

Sample Name :W Peptide, WKYMVm
 Cat No.: RP20299
 Lot No.: E0510119I
 Time Processed :19:43:56
 Month-Day-Year Processed :09/17/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
42.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

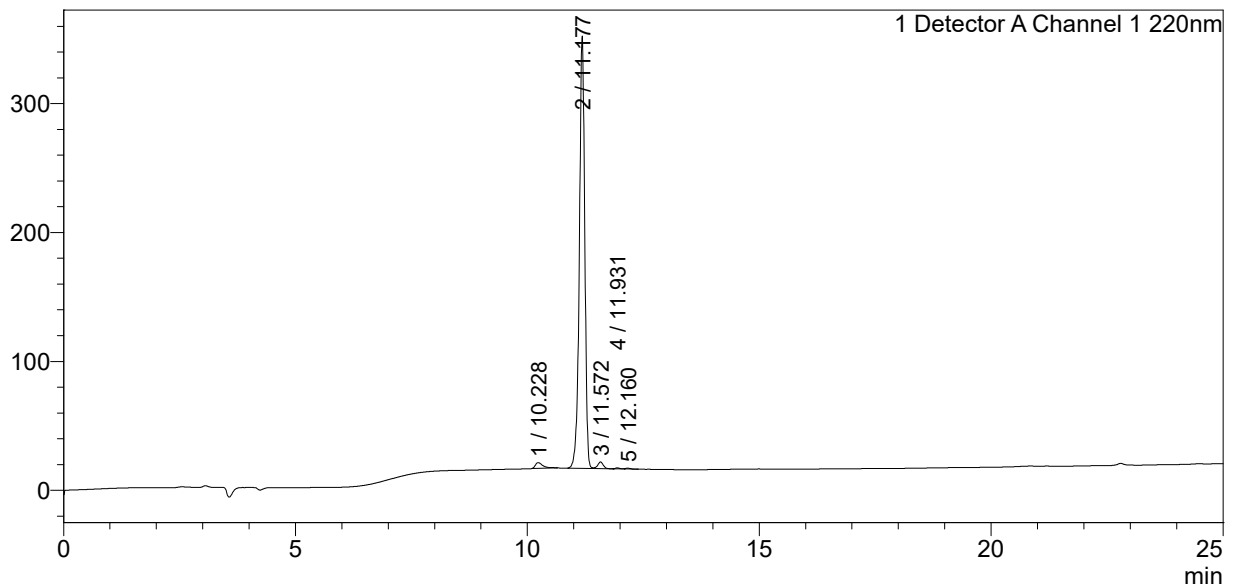

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.228	50602	4518	1.800
2	11.177	2706972	335438	96.316
3	11.572	43403	5172	1.544
4	11.931	5003	764	0.178
5	12.160	4527	694	0.161
Total		2810508	346586	100.000