

Sample Name :HSV-gB2 (498-505)
 Cat. No. : RP19992
 Lot. No. : E1547421G

Time Processed :11:34:53
 Month-Day-Year Processed :07/26/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

| Time | Module | Command | Value |
|-------|------------|---------|-------|
| 0.01 | Pumps | B.Conc | 5 |
| 25.00 | Pumps | B.Conc | 65 |
| 25.01 | Pumps | B.Conc | 95 |
| 27.00 | Pumps | B.Conc | 95 |
| 27.01 | Pumps | B.Conc | 5 |
| 35.00 | Pumps | B.Conc | 5 |
| 35.01 | Controller | Stop | |


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-SP 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

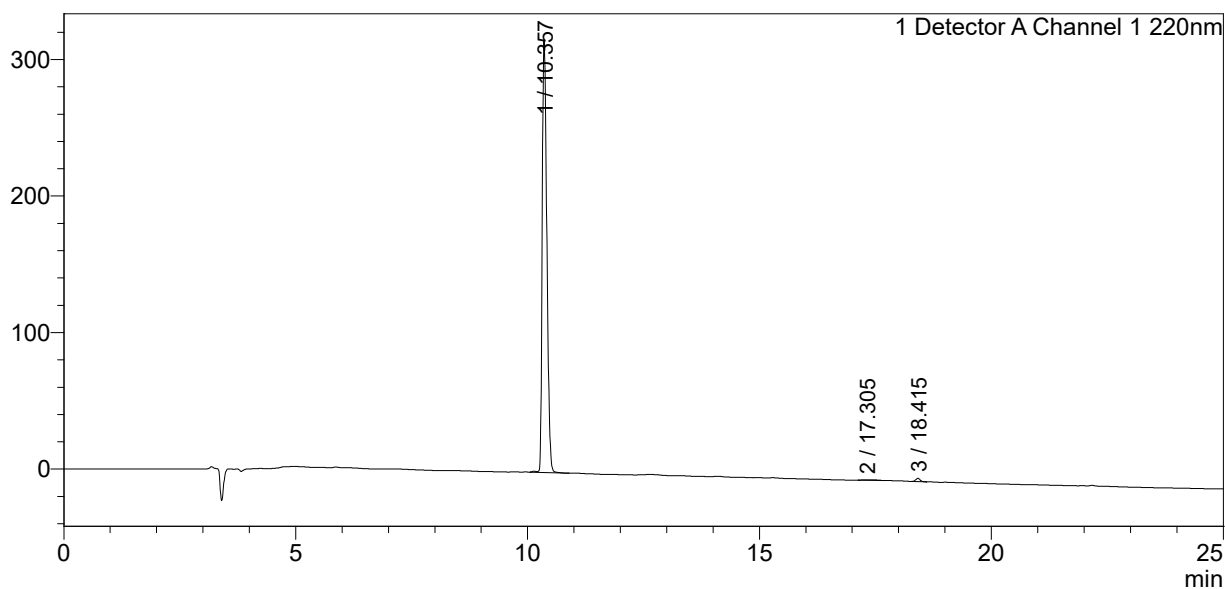

<Peak Table>

Detector A Channel 1 220nm

| Peak# | Ret. Time | Area | Height | Area% |
|-------|-----------|---------|--------|---------|
| 1 | 10.357 | 2204933 | 306703 | 98.933 |
| 2 | 17.305 | 8395 | 422 | 0.377 |
| 3 | 18.415 | 15395 | 2369 | 0.691 |
| Total | | 2228723 | 309494 | 100.000 |