


Mass Spectrum

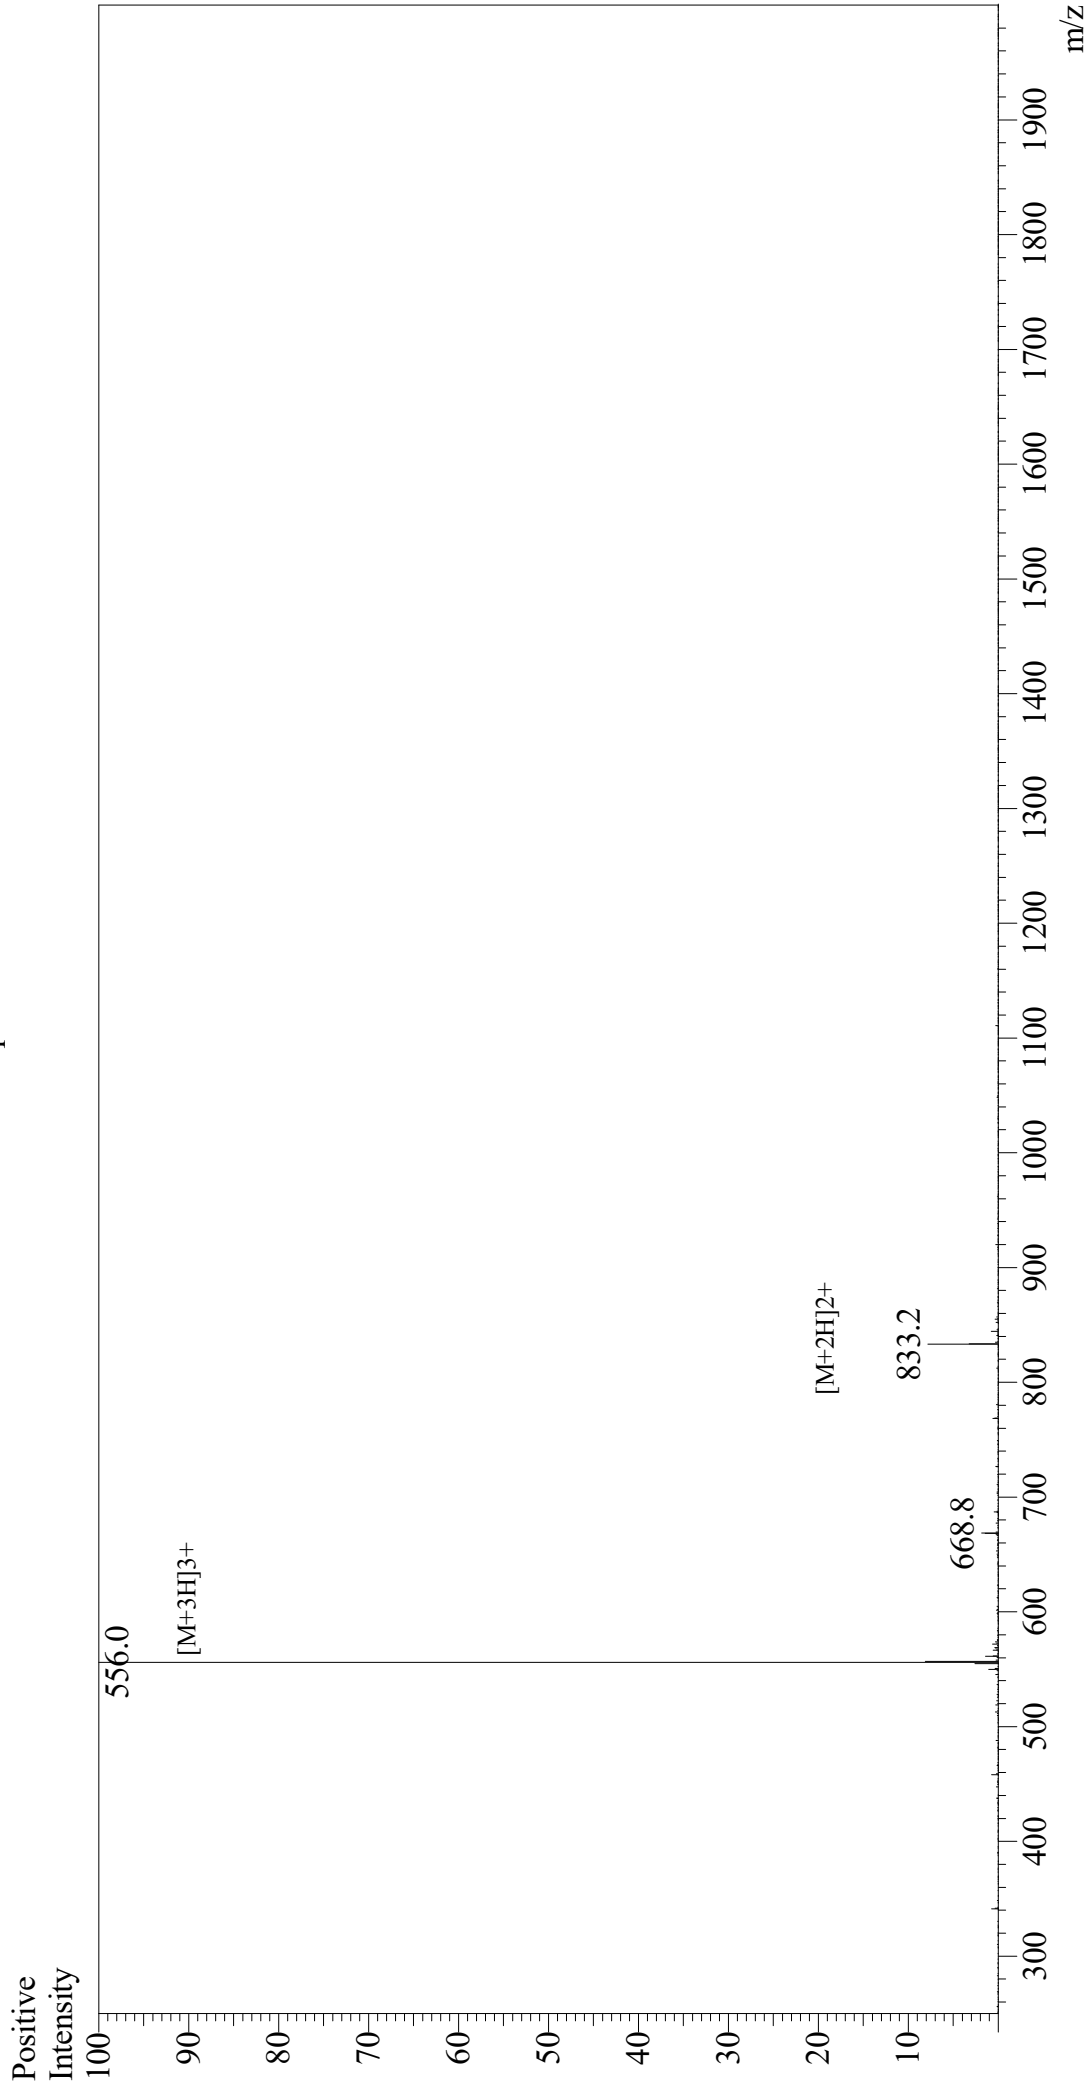

Sample Information  
Month-Day Processed : 09/28/21  
Time Processed : 9:36:52  
Injection Volume : 0.2  
Sample Name :  $\alpha$ -Melanocyte-Stimulating Hormone (MSH), amide  
Cat No. : RP10644  
Lot No. : E01828211  
Theoretical MW : 1664.90  
Observed MW : 1665.0

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : ZJ21010035  
Interface Bias : +4.5 kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2 ml/min  
B.conc : 50%H<sub>2</sub>O/50%MeOH