

Sample Name : N-Boc-Phe-Leu-Phe-Leu-Phe
 Cat. No. : RP12950
 Lot. No. : E8074421C
 Time Processed : 20:34:06
 Month-Day-Year Processed : 03/18/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
45.00	Pumps	Pump A B.Conc	5
72.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

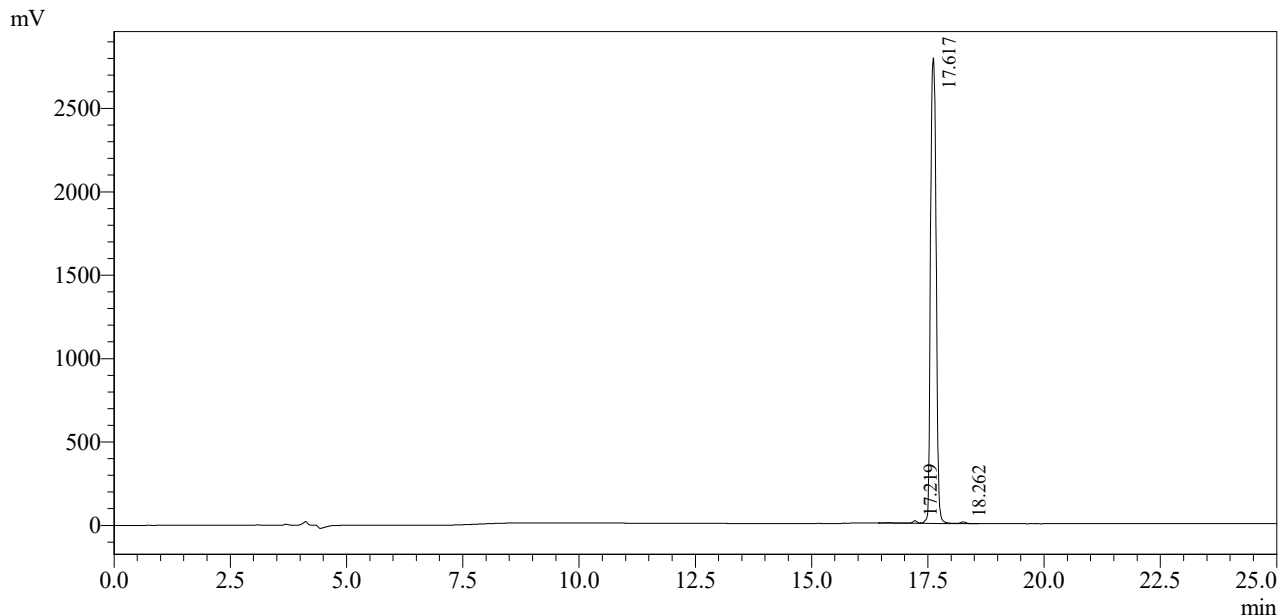

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.219	171231	16001	0.722
2	17.617	23439410	2791345	98.785
3	18.262	117081	10312	0.493
Total		23727721	2817658	100.000