

Sample Name: Octreotide (SMS 201-995)
 Cat No. : RP10222
 Lot No. : E2782820E
 Time Processed: 6:01:19 AM
 Month-Day-Year Processed :05/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

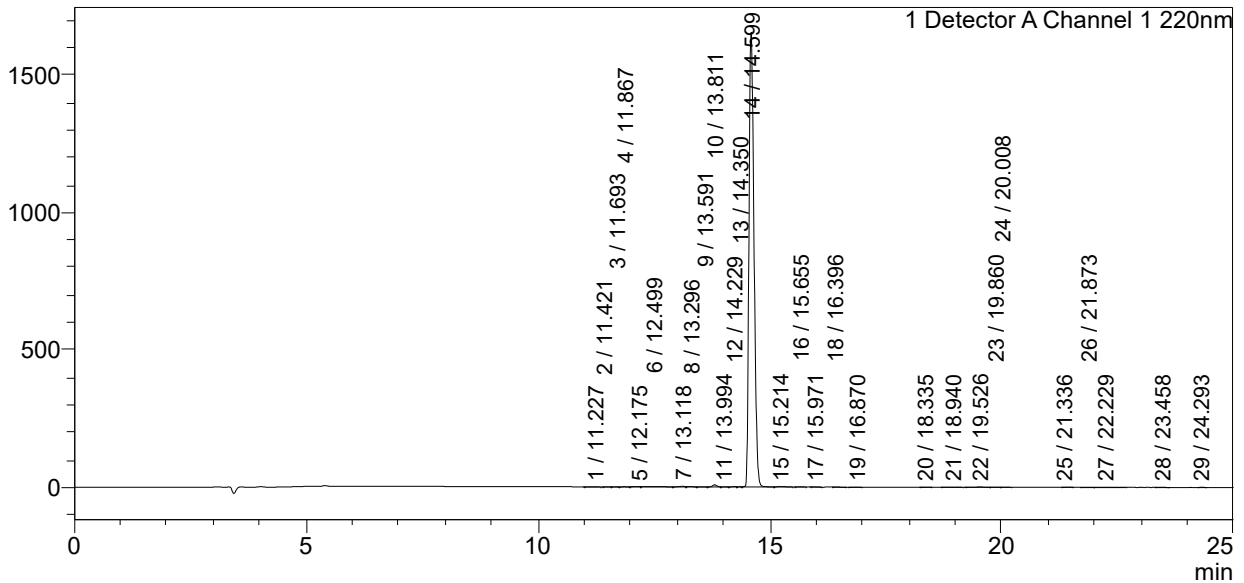

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.227	2057	162	0.016
2	11.421	1650	163	0.013
3	11.693	1383	203	0.011
4	11.867	3683	293	0.029
5	12.175	5100	419	0.040
6	12.499	31080	1260	0.245
7	13.118	16762	1939	0.132
8	13.296	9680	1568	0.076
9	13.591	3865	448	0.030
10	13.811	48532	7662	0.383
11	13.994	3525	546	0.028
12	14.229	6764	884	0.053
13	14.350	3318	701	0.026
14	14.599	12465012	1655140	98.294

Peak#	Ret. Time	Area	Height	Area%
15	15.214	20034	1813	0.158
16	15.655	1505	270	0.012
17	15.971	3506	554	0.028
18	16.396	2149	188	0.017
19	16.870	1416	141	0.011
20	18.335	1236	134	0.010
21	18.940	4136	265	0.033
22	19.526	15440	1075	0.122
23	19.860	4825	467	0.038
24	20.008	2671	335	0.021
25	21.336	1011	121	0.008
26	21.873	3184	286	0.025
27	22.229	15059	635	0.119
28	23.458	1578	170	0.012
29	24.293	1211	161	0.010
Total		12681372	1678003	100.000