

Sample Name : Hepatitis B Virus Core (128-140)
 Cat. No. : RP17313
 Lot. No. : PE4121707

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

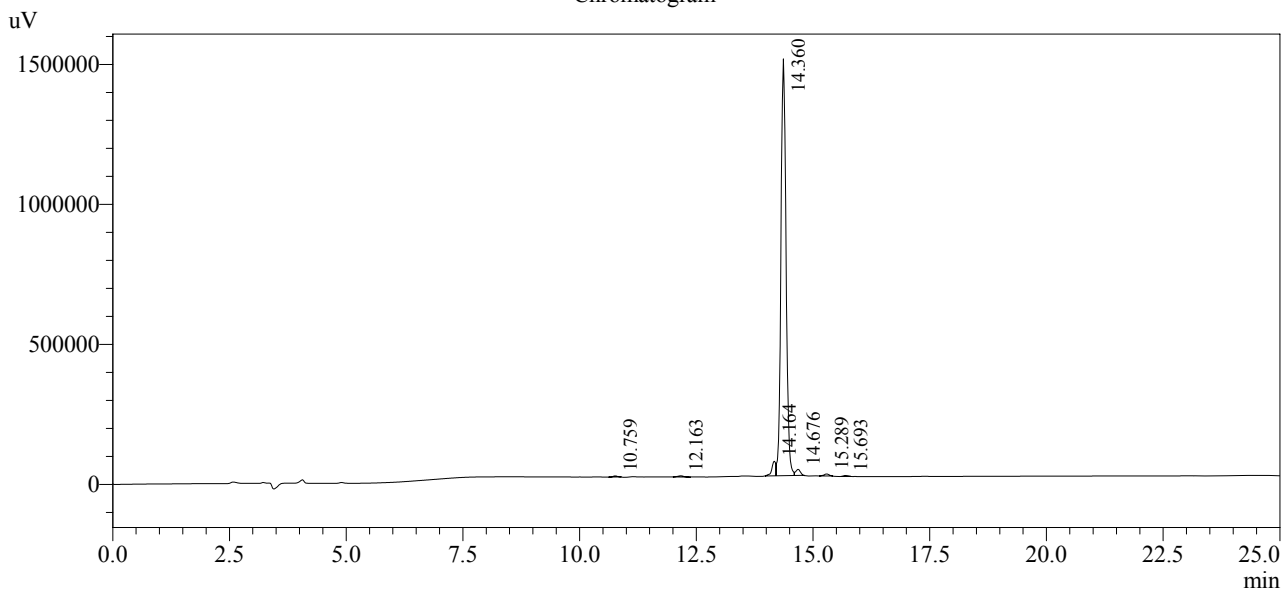

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.759	23610	3862	0.198
2	12.163	34298	3947	0.287
3	14.164	307098	51896	2.572
4	14.360	11359430	1488462	95.138
5	14.676	148916	21501	1.247
6	15.289	50343	6899	0.422
7	15.693	16235	2785	0.136
Total		11939929	1579351	100.000