

Sample Name :Indolicidin  
 Cat. No. : RP11242  
 Lot. No. :E0909019G  
 Time Processed :7:33:30  
 Month-Day-Year Processed :07/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

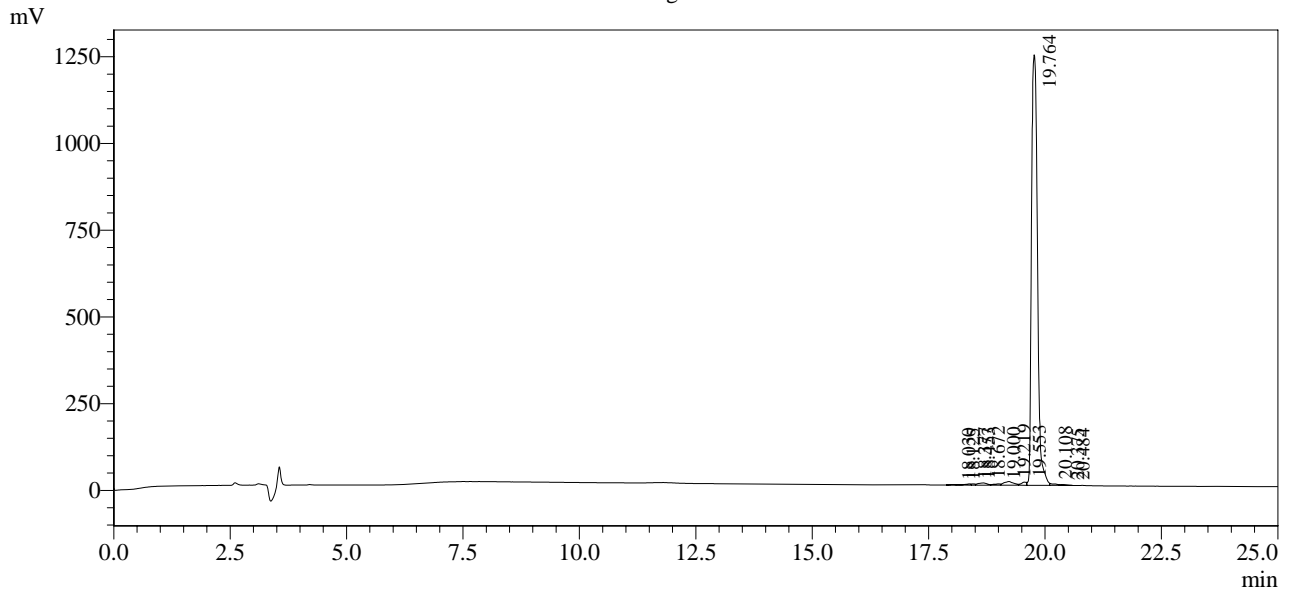

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.030	7831	966	0.068
2	18.125	2676	644	0.023
3	18.377	30468	3442	0.264
4	18.453	18380	3667	0.159
5	18.672	85347	6552	0.740
6	19.000	38353	3941	0.333
7	19.219	154361	10776	1.339
8	19.553	70249	8872	0.609
9	19.764	11055951	1240706	95.876
10	20.108	43842	5546	0.380
11	20.375	17889	2636	0.155
12	20.484	6157	1284	0.053
Total		11531504	1289032	100.000